




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
Data File : BN030162.D
Acq On : 29 Feb 2024 11:14
Operator : MA/JU
Sample : P1535-02
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC6

Manual IntegrationsAPPROVED

Quant Time: Feb 29 11:51:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 23:49:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/29/2024
Supervised By :mohammad ahmed 03/01/2024

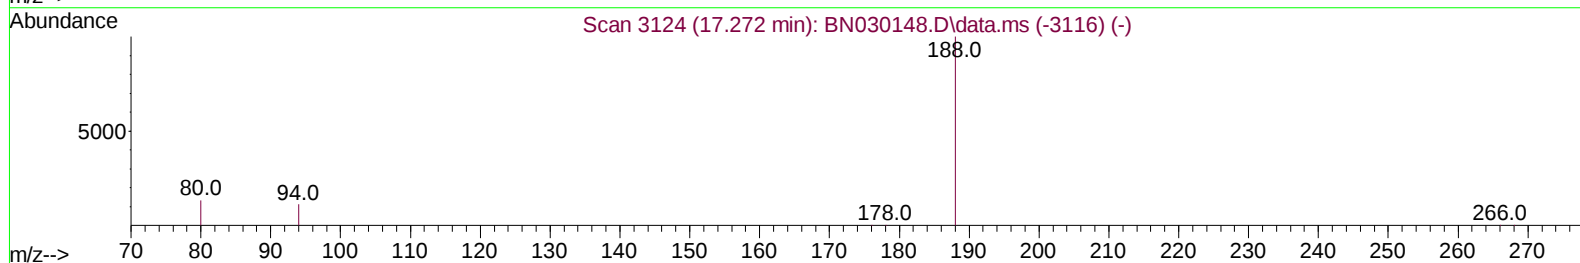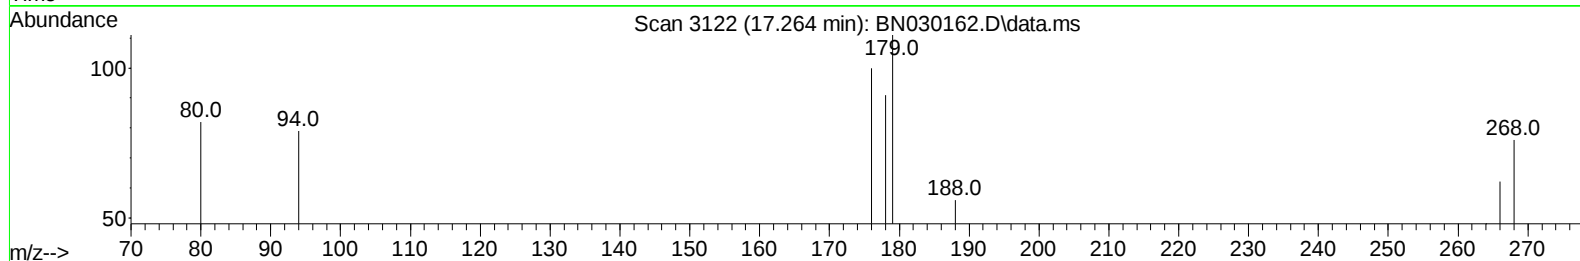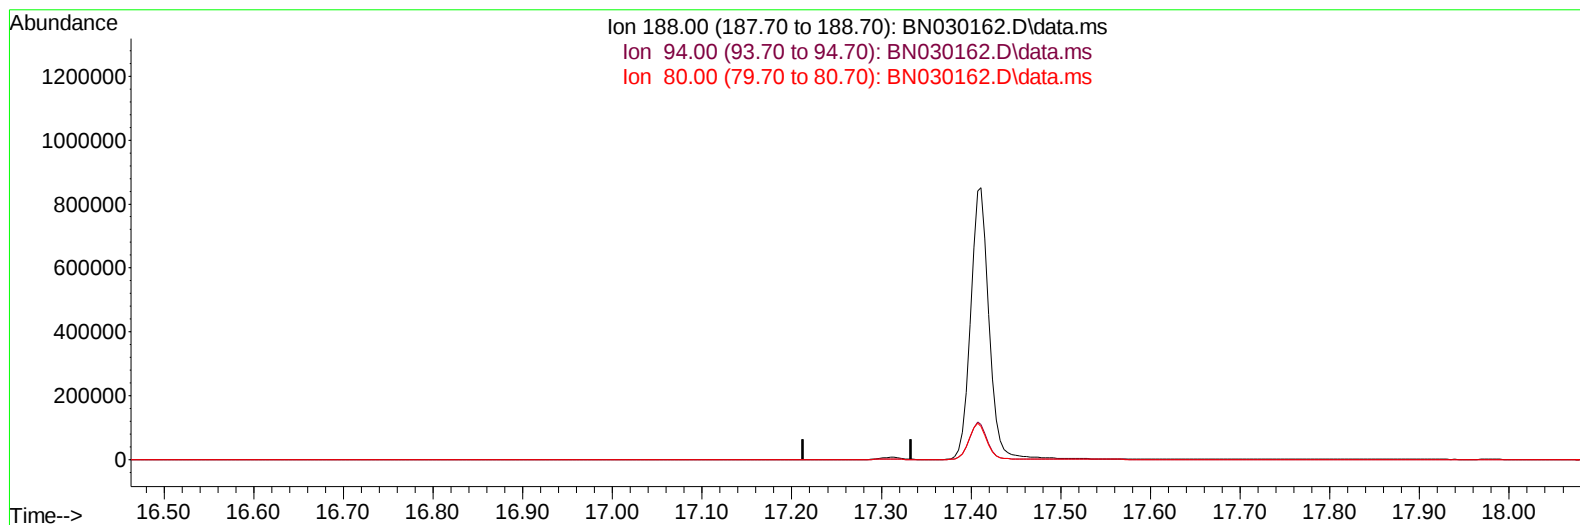

TIC: BN030162.D\data.ms

(13) Phenanthrene-d10 (I)

17.263min (-17.263) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	12.00	0.00#
80.00	13.70	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
Data File : BN030162.D
Acq On : 29 Feb 2024 11:14
Operator : MA/JU
Sample : P1535-02
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC6

Manual IntegrationsAPPROVED

Quant Time: Feb 29 11:51:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 23:49:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/29/2024
Supervised By :mohammad ahmed 03/01/2024

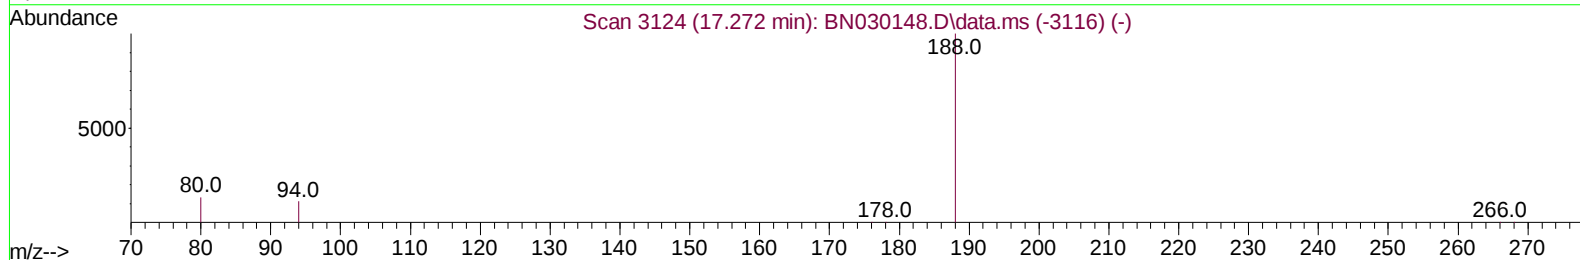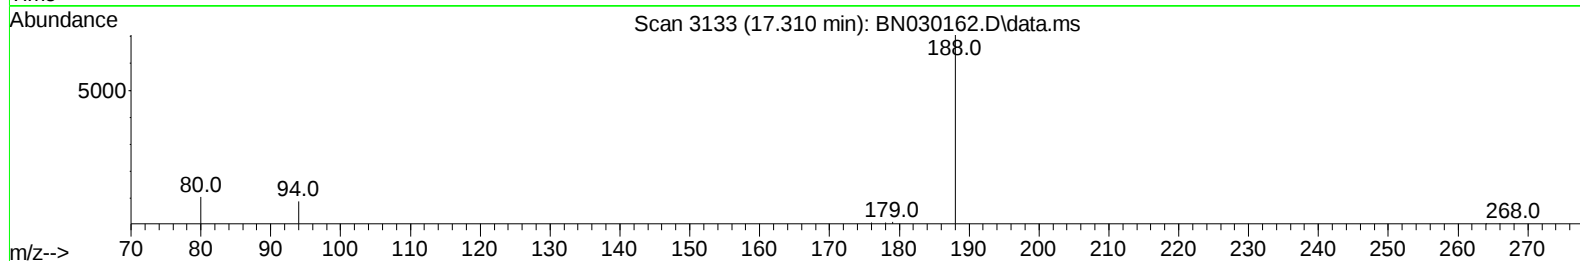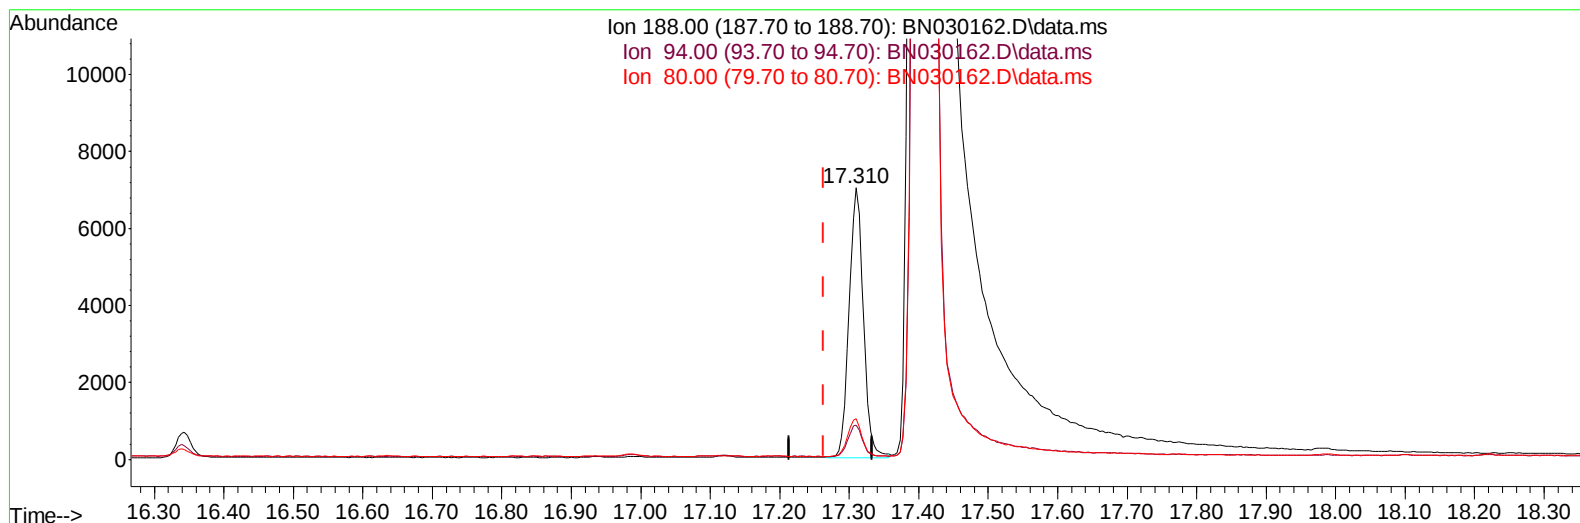

TIC: BN030162.D\data.ms

(13) Phenanthrene-d10 (I)

17.310min (+ 0.047) 0.40 ng/ul m

response 10018

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.00	12.60
80.00	13.70	14.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
 Data File : BN030162.D
 Acq On : 29 Feb 2024 11:14
 Operator : MA/JU
 Sample : P1535-02
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC6

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/29/2024
 Supervised By :mohammad ahmed 03/01/2024

Quant Time: Feb 29 11:51:06 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 27 23:49:29 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.922	152		4045	0.400	ng/ul	0.07
4) Naphthalene-d8	10.722	136		6669	0.400	ng/ul	0.07
9) Acenaphthene-d10	14.562	164		3682	0.400	ng/ul	# 0.07
13) Phenanthrene-d10	17.310	188		10018m	0.400	ng/ul	0.05
17) Chrysene-d12	21.508	240		6338	0.400	ng/ul	0.04
23) Perylene-d12	23.905	264		5847	0.400	ng/ul	0.08
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.345	96		21644	4.291	ng/ul	0.03
6) 2-Methylnaphthalene-d10	12.322	152		3932	0.463	ng/ul	0.08
18) Fluoranthene-d10	19.341	212		12918	0.620	ng/ul	0.05
Target Compounds							Qvalue
2) 1,4-Dioxane	3.382	88		4448	0.810	ng/ul	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
Data File : BN030162.D
Acq On : 29 Feb 2024 11:14
Operator : MA/JU
Sample : P1535-02
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC6

Manual IntegrationsAPPROVED

Quant Time: Feb 29 11:51:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 23:49:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/29/2024
Supervised By :mohammad ahmed 03/01/2024

