

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
 Data File : BN030101.D
 Acq On : 27 Feb 2024 20:43
 Operator : MA/JU
 Sample : P1508-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH403

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 02/28/2024
 Supervised By :mohammad ahmed 03/01/2024

Quant Time: Feb 27 23:51:33 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 27 23:49:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.850	152	4122	0.400	ng/ul	0.00
4) Naphthalene-d8	10.643	136	12054	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.496	164	5819	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.249	188	10897	0.400	ng/ul	-0.01
17) Chrysene-d12	21.455	240	7010	0.400	ng/ul	-0.01
23) Perylene-d12	23.802	264	10494m	0.400	ng/ul	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.315	96	22901	4.456	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.243	152	6113	0.399	ng/ul	0.00
18) Fluoranthene-d10	19.283	212	11989	0.520	ng/ul	-0.01
Target Compounds					Qvalue	
2) 1,4-Dioxane	3.353	88	373	0.067	ng/ul#	69

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
Data File : BN030101.D
Acq On : 27 Feb 2024 20:43
Operator : MA/JU
Sample : P1508-05
Misc :
ALS Vial : 6 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
BH403

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 02/28/2024
Supervised By :mohammad ahmed 03/01/2024


Quant Time: Feb 27 23:51:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 23:49:29 2024
Response via : Initial Calibration

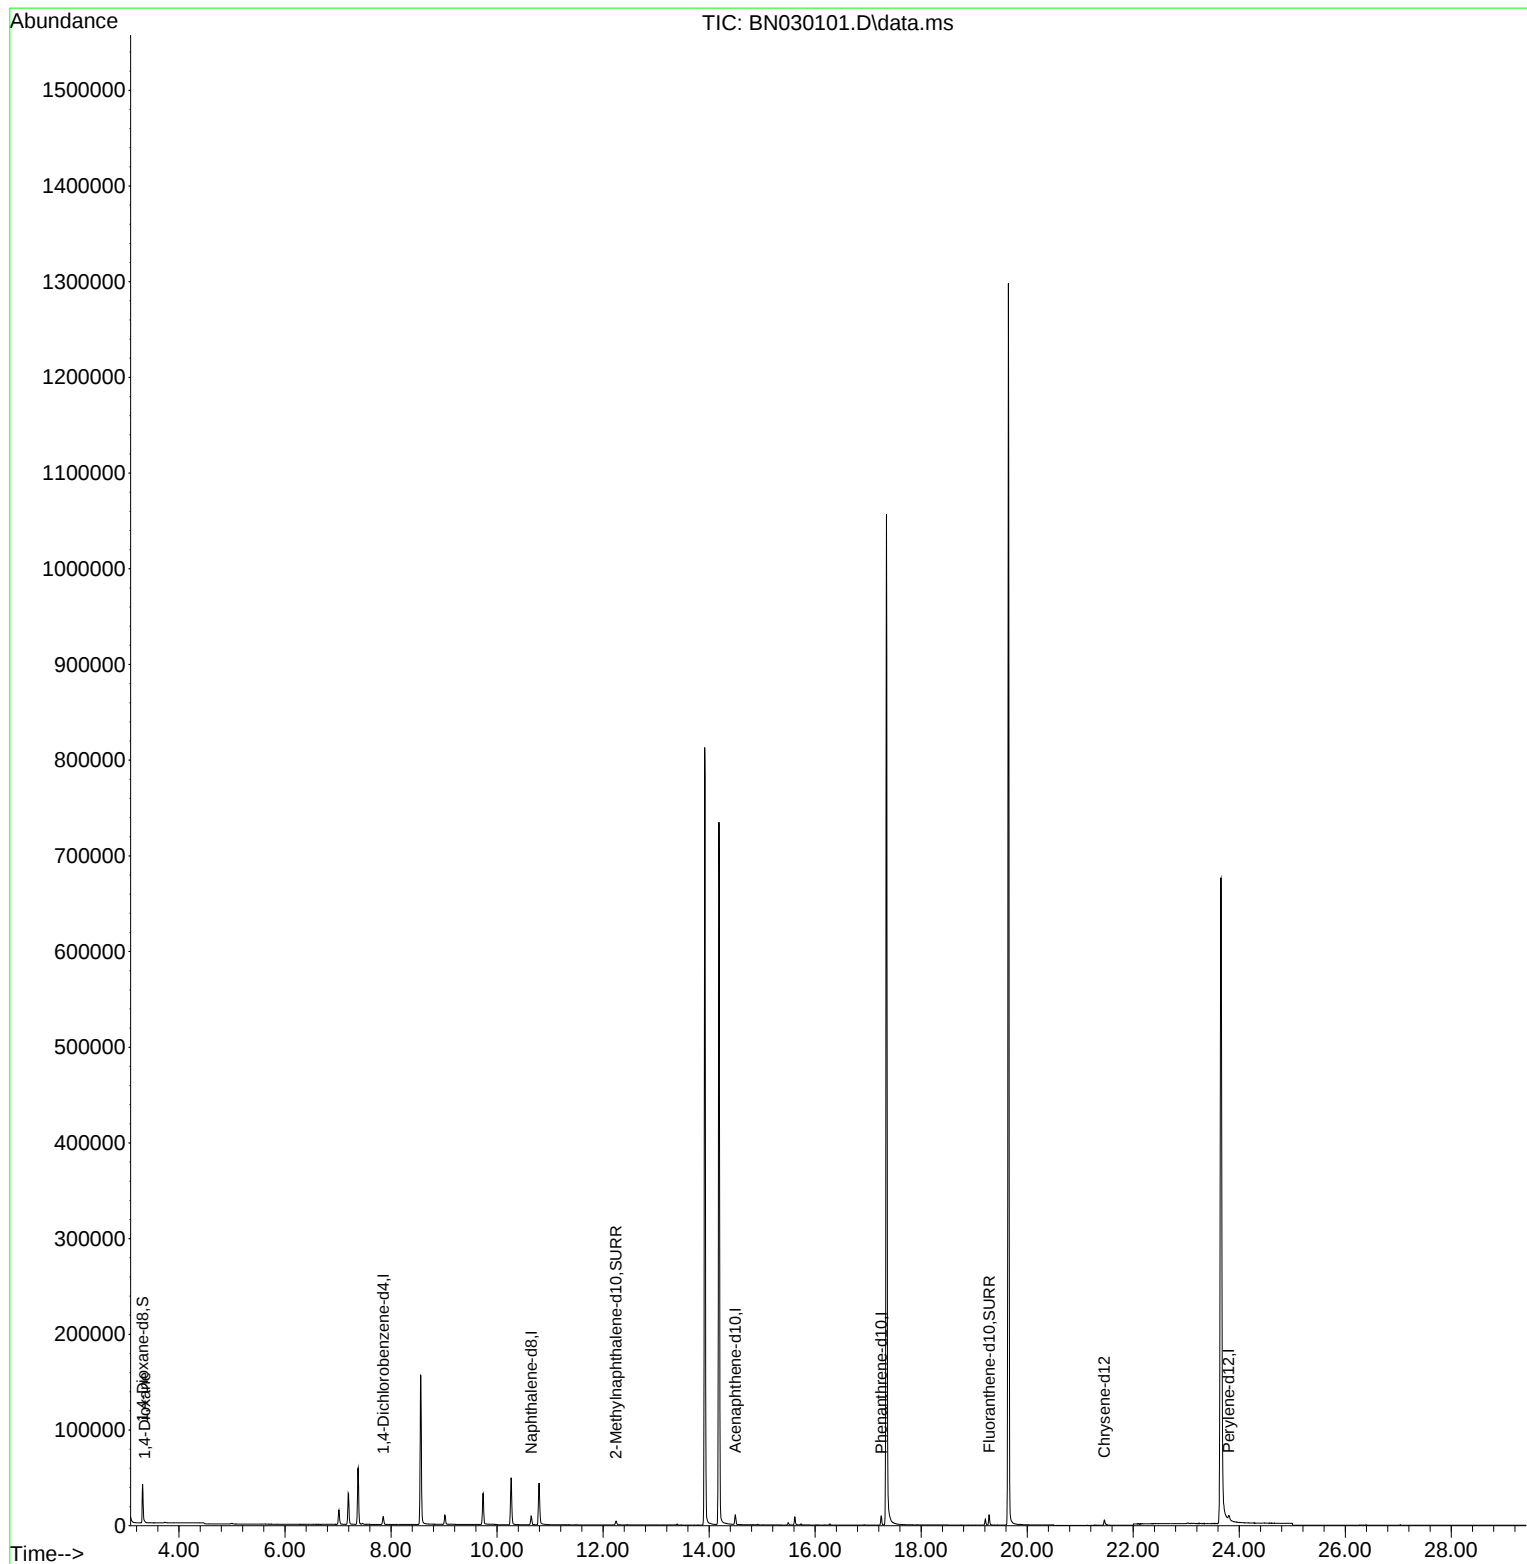

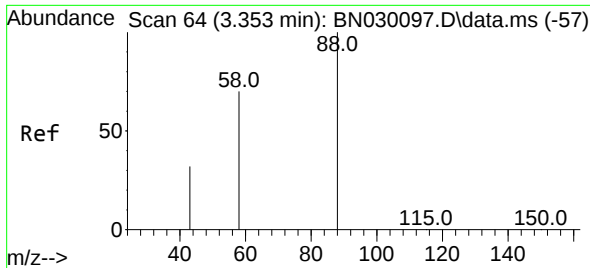

#2
 1,4-Dioxane
 Concen: 0.067 ng/ul
 RT: 3.353 min Scan# 64
 Delta R.T. -0.000 min
 Lab File: BN030101.D
 Acq: 27 Feb 2024 20:43

Instrument :
 BNA_N
 ClientSampleId :
 BH403

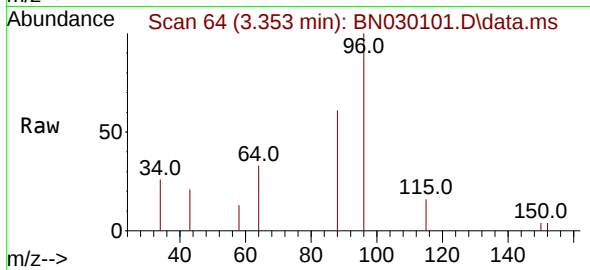

Tgt Ion: 88 Resp: 37

Ion	Ratio	Lower	Upper
88	100		
43	34.7	21.8	32.6
58	21.9	39.3	58.9

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 02/28/2024
 Supervised By :mohammad ahmed 03/01/2024

