

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
 Data File : BN030109.D
 Acq On : 28 Feb 2024 01:33
 Operator : MA/JU
 Sample : P1526-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E10B7

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 02/28/2024
 Supervised By :mohammad ahmed 03/01/2024

Quant Time: Feb 28 01:59:47 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 27 23:49:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.851	152	3910	0.400	ng/ul	0.00
4) Naphthalene-d8	10.643	136	11194	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.496	164	5663	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.245	188	11324	0.400	ng/ul	-0.02
17) Chrysene-d12	21.452	240	8458	0.400	ng/ul	-0.01
23) Perylene-d12	23.799	264	5985m	0.400	ng/ul	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.315	96	21374	4.384	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.244	152	5947	0.418	ng/ul	0.00
18) Fluoranthene-d10	19.279	212	13725	0.494	ng/ul	-0.02
Target Compounds						Qvalue
5) Naphthalene	10.693	128	806	0.026	ng/ul#	72

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
Data File : BN030109.D
Acq On : 28 Feb 2024 01:33
Operator : MA/JU
Sample : P1526-05
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
E10B7

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 02/28/2024
Supervised By :mohammad ahmed 03/01/2024


Quant Time: Feb 28 01:59:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 23:49:29 2024
Response via : Initial Calibration

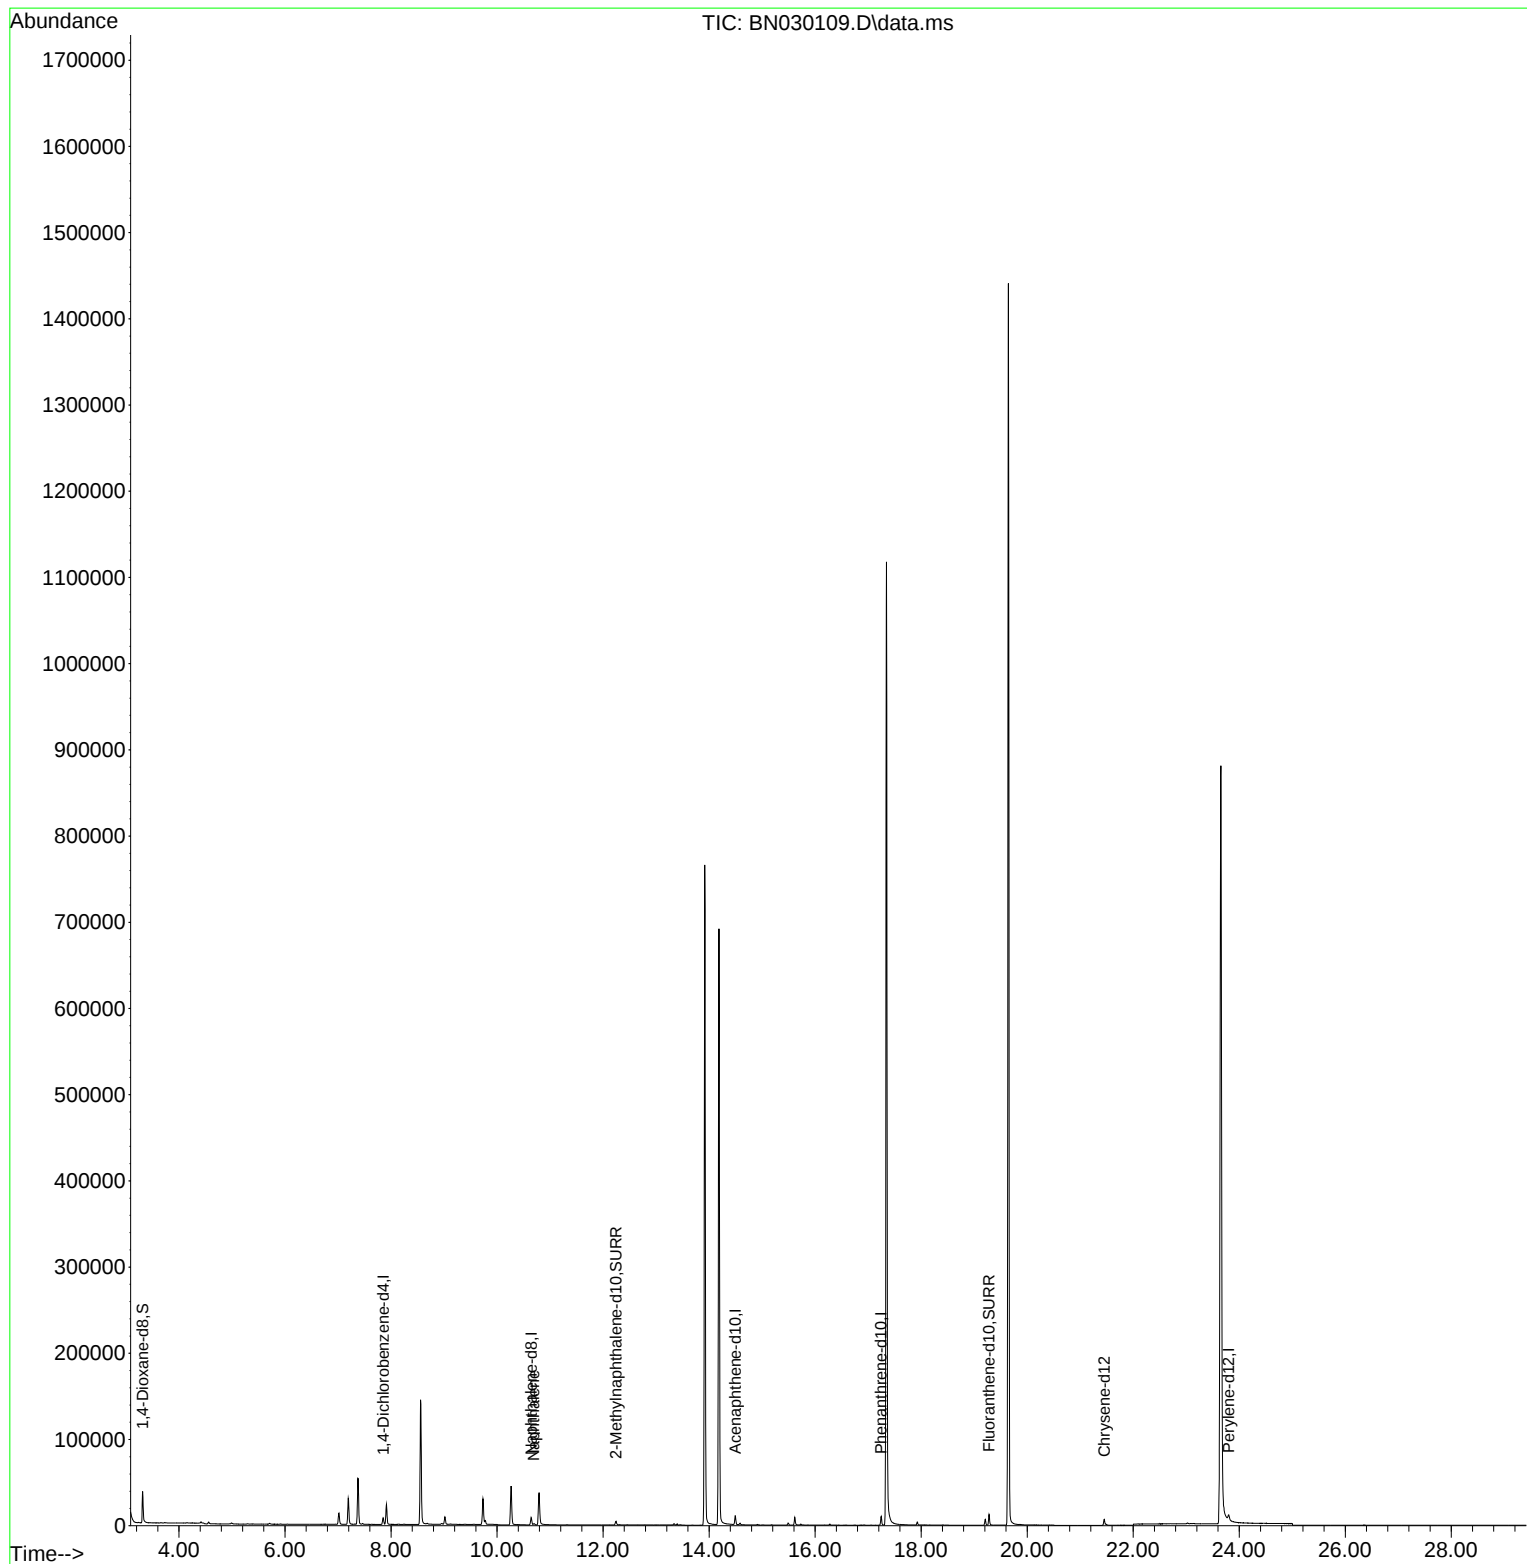

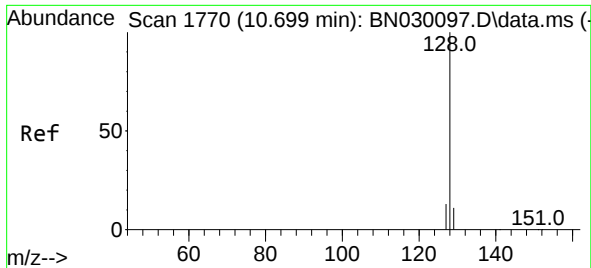

#5
Naphthalene
Concen: 0.026 ng/ul
RT: 10.693 min Scan# 1770
Delta R.T. -0.006 min
Lab File: BN030109.D
Acq: 28 Feb 2024 01:33

Instrument :
BNA_N
ClientSampleId :
E10B7

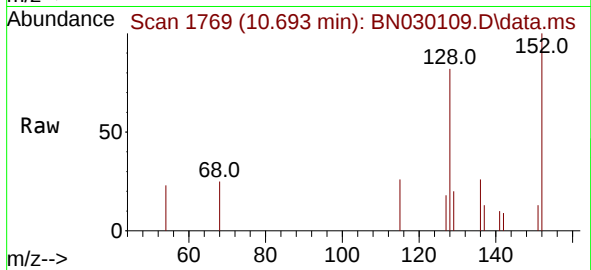

Tgt Ion:128 Resp: 800
Ion Ratio Lower Upper
128 100
129 24.6 9.1 13.7
127 22.6 11.0 16.6

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 02/28/2024
Supervised By :mohammad ahmed 03/01/2024

