

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
 Data File : BN030124.D
 Acq On : 28 Feb 2024 11:13
 Operator : MA/JU
 Sample : P1498-01
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AB6

Quant Time: Feb 28 11:45:08 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 27 23:49:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.851	152	5359	0.400	ng/ul	0.00
4) Naphthalene-d8	10.645	136	15316	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.493	164	7562	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.247	188	14456	0.400	ng/ul	-0.02
17) Chrysene-d12	21.454	240	9553	0.400	ng/ul	-0.01
23) Perylene-d12	23.807	264	11183	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.315	96	29245	4.377	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.240	152	8048	0.413	ng/ul	0.00
18) Fluoranthene-d10	19.281	212	13405	0.427	ng/ul	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.340	88	722	0.099	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
Data File : BN030124.D
Acq On : 28 Feb 2024 11:13
Operator : MA/JU
Sample : P1498-01
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AB6

Quant Time: Feb 28 11:45:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 23:49:29 2024
Response via : Initial Calibration

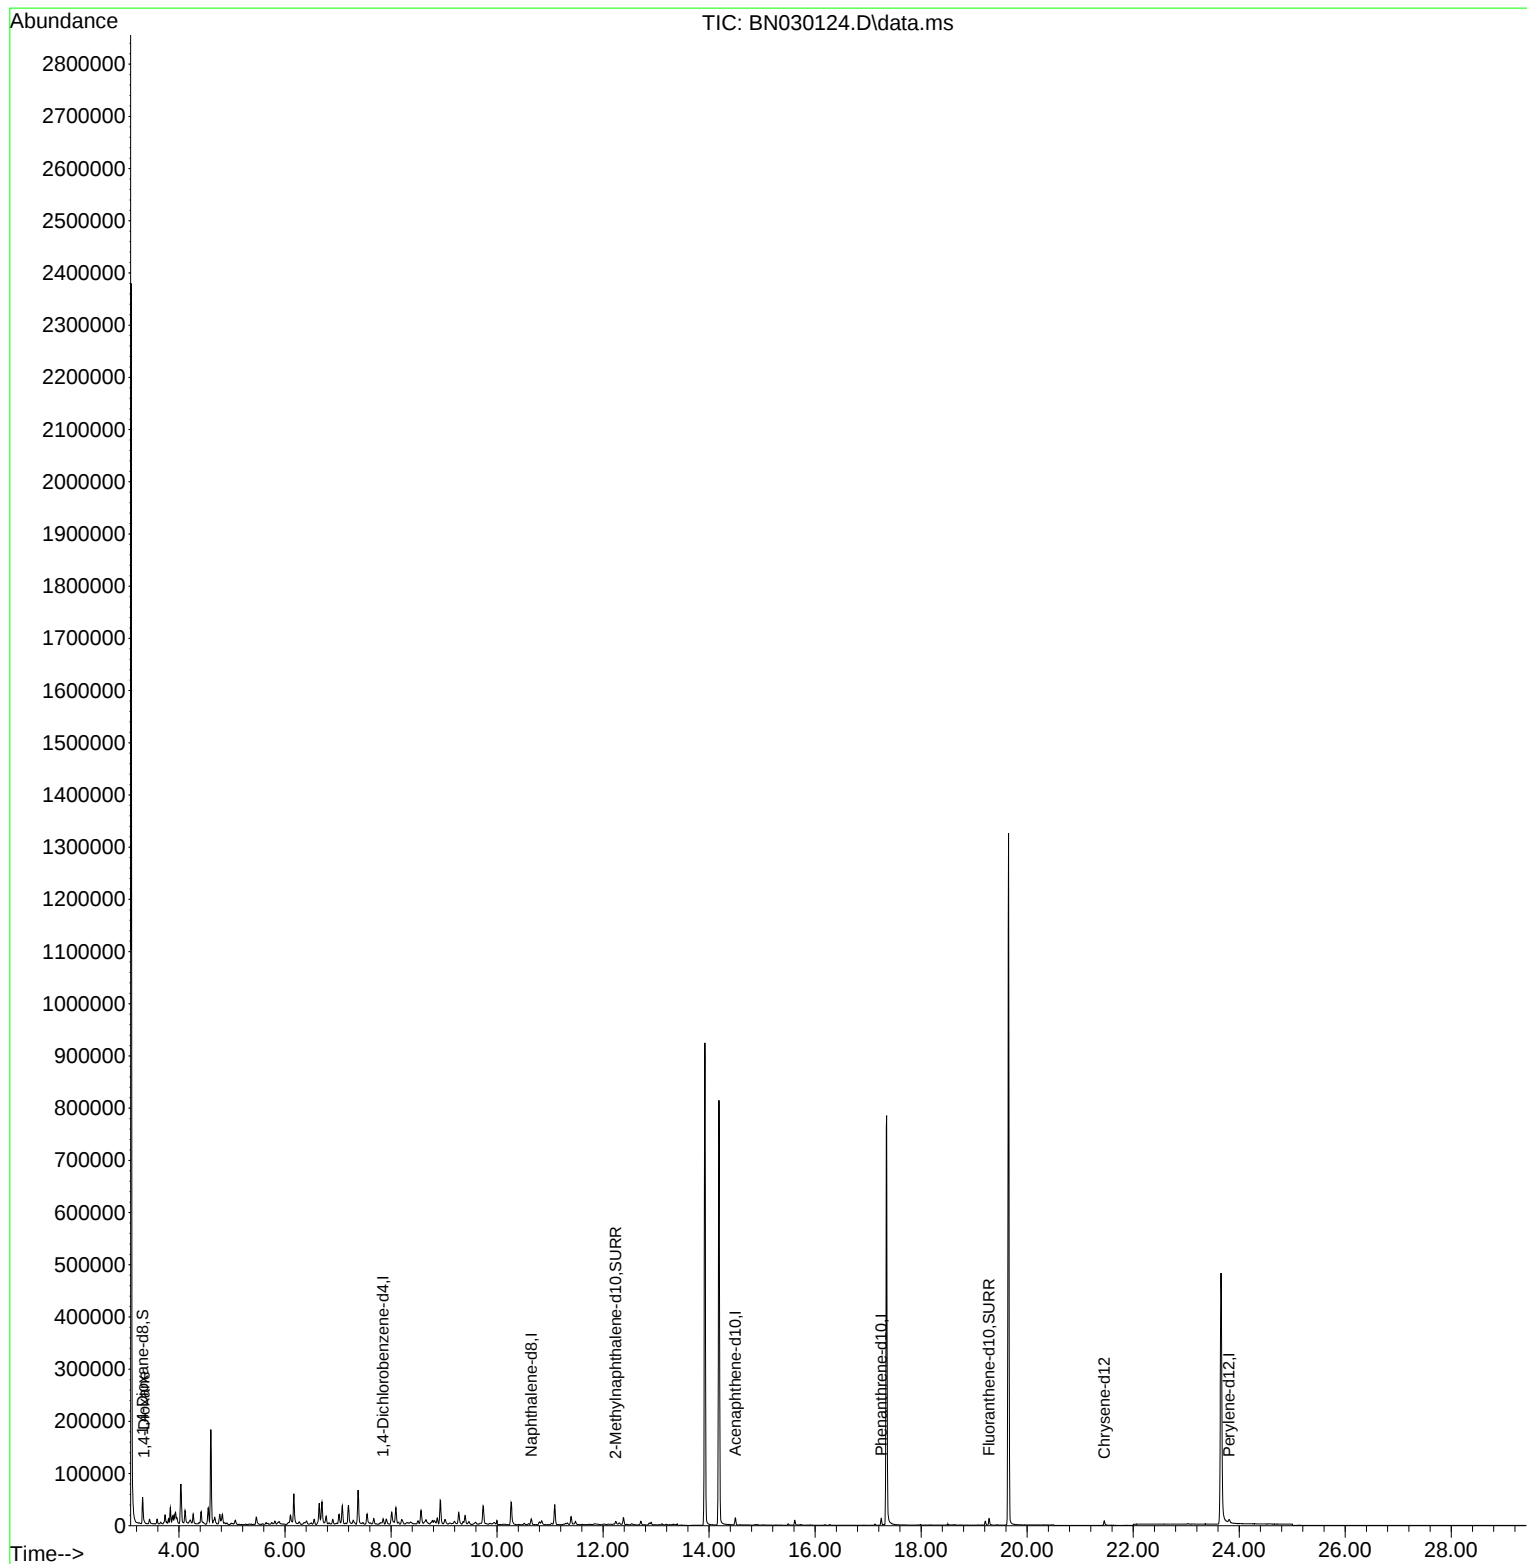

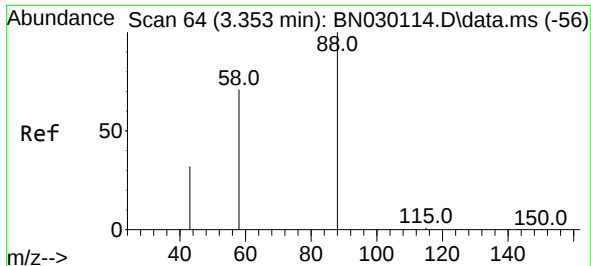

#2
 1,4-Dioxane
 Concen: 0.099 ng/ul
 RT: 3.340 min Scan# 61
 Delta R.T. -0.012 min
 Lab File: BN030124.D
 Acq: 28 Feb 2024 11:13

Instrument :
 BNA_N
 ClientSampleId :
 C0AB6

Tgt Ion: 88 Resp: 722
 Ion Ratio Lower Upper
 88 100
 43 293.1 21.8 32.6#
 58 28.7 39.3 58.9#

