

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
 Data File : BN030126.D
 Acq On : 28 Feb 2024 12:25
 Operator : MA/JU
 Sample : P1498-11
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AB2

Quant Time: Feb 28 13:11:03 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 27 23:49:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.851	152	6058	0.400	ng/ul	0.00
4) Naphthalene-d8	10.645	136	18395	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.493	164	7706	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.247	188	21095	0.400	ng/ul	-0.02
17) Chrysene-d12	21.453	240	12624	0.400	ng/ul	-0.01
23) Perylene-d12	23.806	264	12673	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.315	96	34716	4.596	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.240	152	12902	0.551	ng/ul	0.00
18) Fluoranthene-d10	19.282	212	26222	0.632	ng/ul	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.349	88	6439	0.783	ng/ul#	33


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
Data File : BN030126.D
Acq On : 28 Feb 2024 12:25
Operator : MA/JU
Sample : P1498-11
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AB2


Quant Time: Feb 28 13:11:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 23:49:29 2024
Response via : Initial Calibration

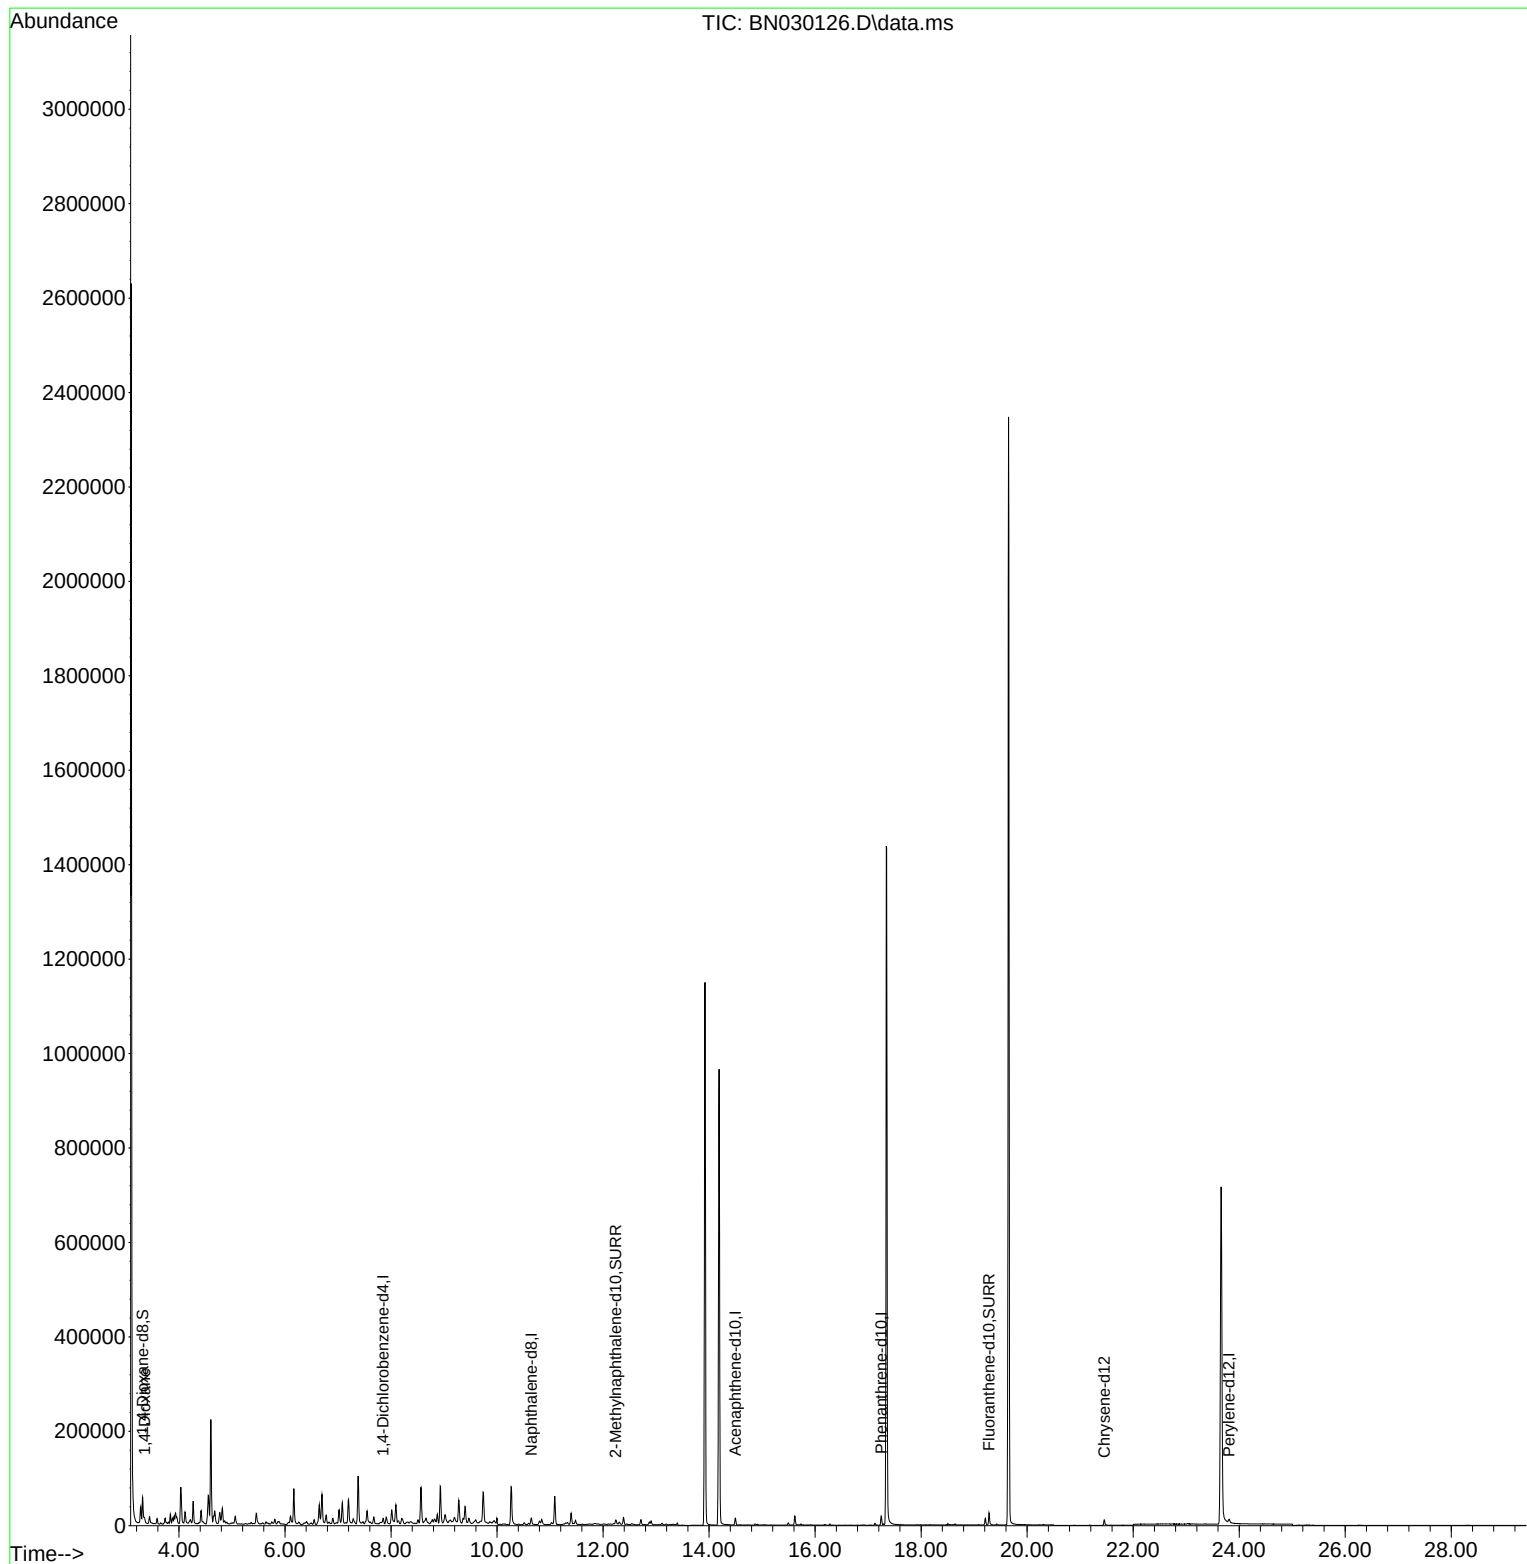

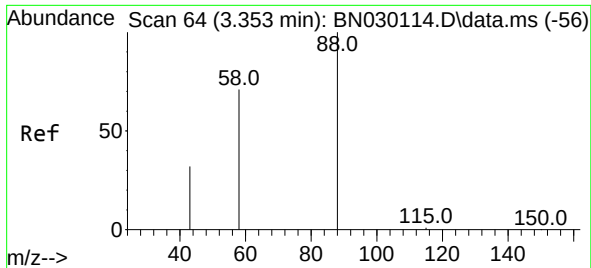

#2
 1,4-Dioxane
 Concen: 0.783 ng/ul
 RT: 3.349 min Scan# 61
 Delta R.T. -0.004 min
 Lab File: BN030126.D
 Acq: 28 Feb 2024 12:25

Instrument :
 BNA_N
 ClientSampleId :
 C0AB2

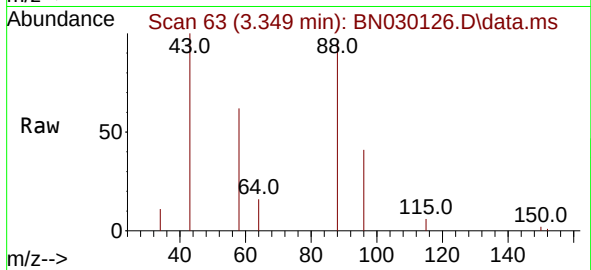

Tgt Ion:	88	Resp:	6439
Ion	Ratio	Lower	Upper
88	100		
43	103.9	21.8	32.6#
58	64.4	39.3	58.9#

