

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
 Data File : BN030127.D
 Acq On : 28 Feb 2024 13:01
 Operator : MA/JU
 Sample : P1498-12
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AB3

Quant Time: Feb 28 14:03:59 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 27 23:49:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.851	152	5743	0.400	ng/ul	0.00
4) Naphthalene-d8	10.645	136	15931	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.497	164	7939	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.247	188	14471	0.400	ng/ul	-0.02
17) Chrysene-d12	21.452	240	11861	0.400	ng/ul	-0.01
23) Perylene-d12	23.811	264	13966	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.315	96	35312	4.931	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.240	152	9976	0.492	ng/ul	0.00
18) Fluoranthene-d10	19.281	212	17462	0.448	ng/ul	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.353	88	5807	0.745	ng/ul#	54


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
Data File : BN030127.D
Acq On : 28 Feb 2024 13:01
Operator : MA/JU
Sample : P1498-12
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AB3

Quant Time: Feb 28 14:03:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 23:49:29 2024
Response via : Initial Calibration

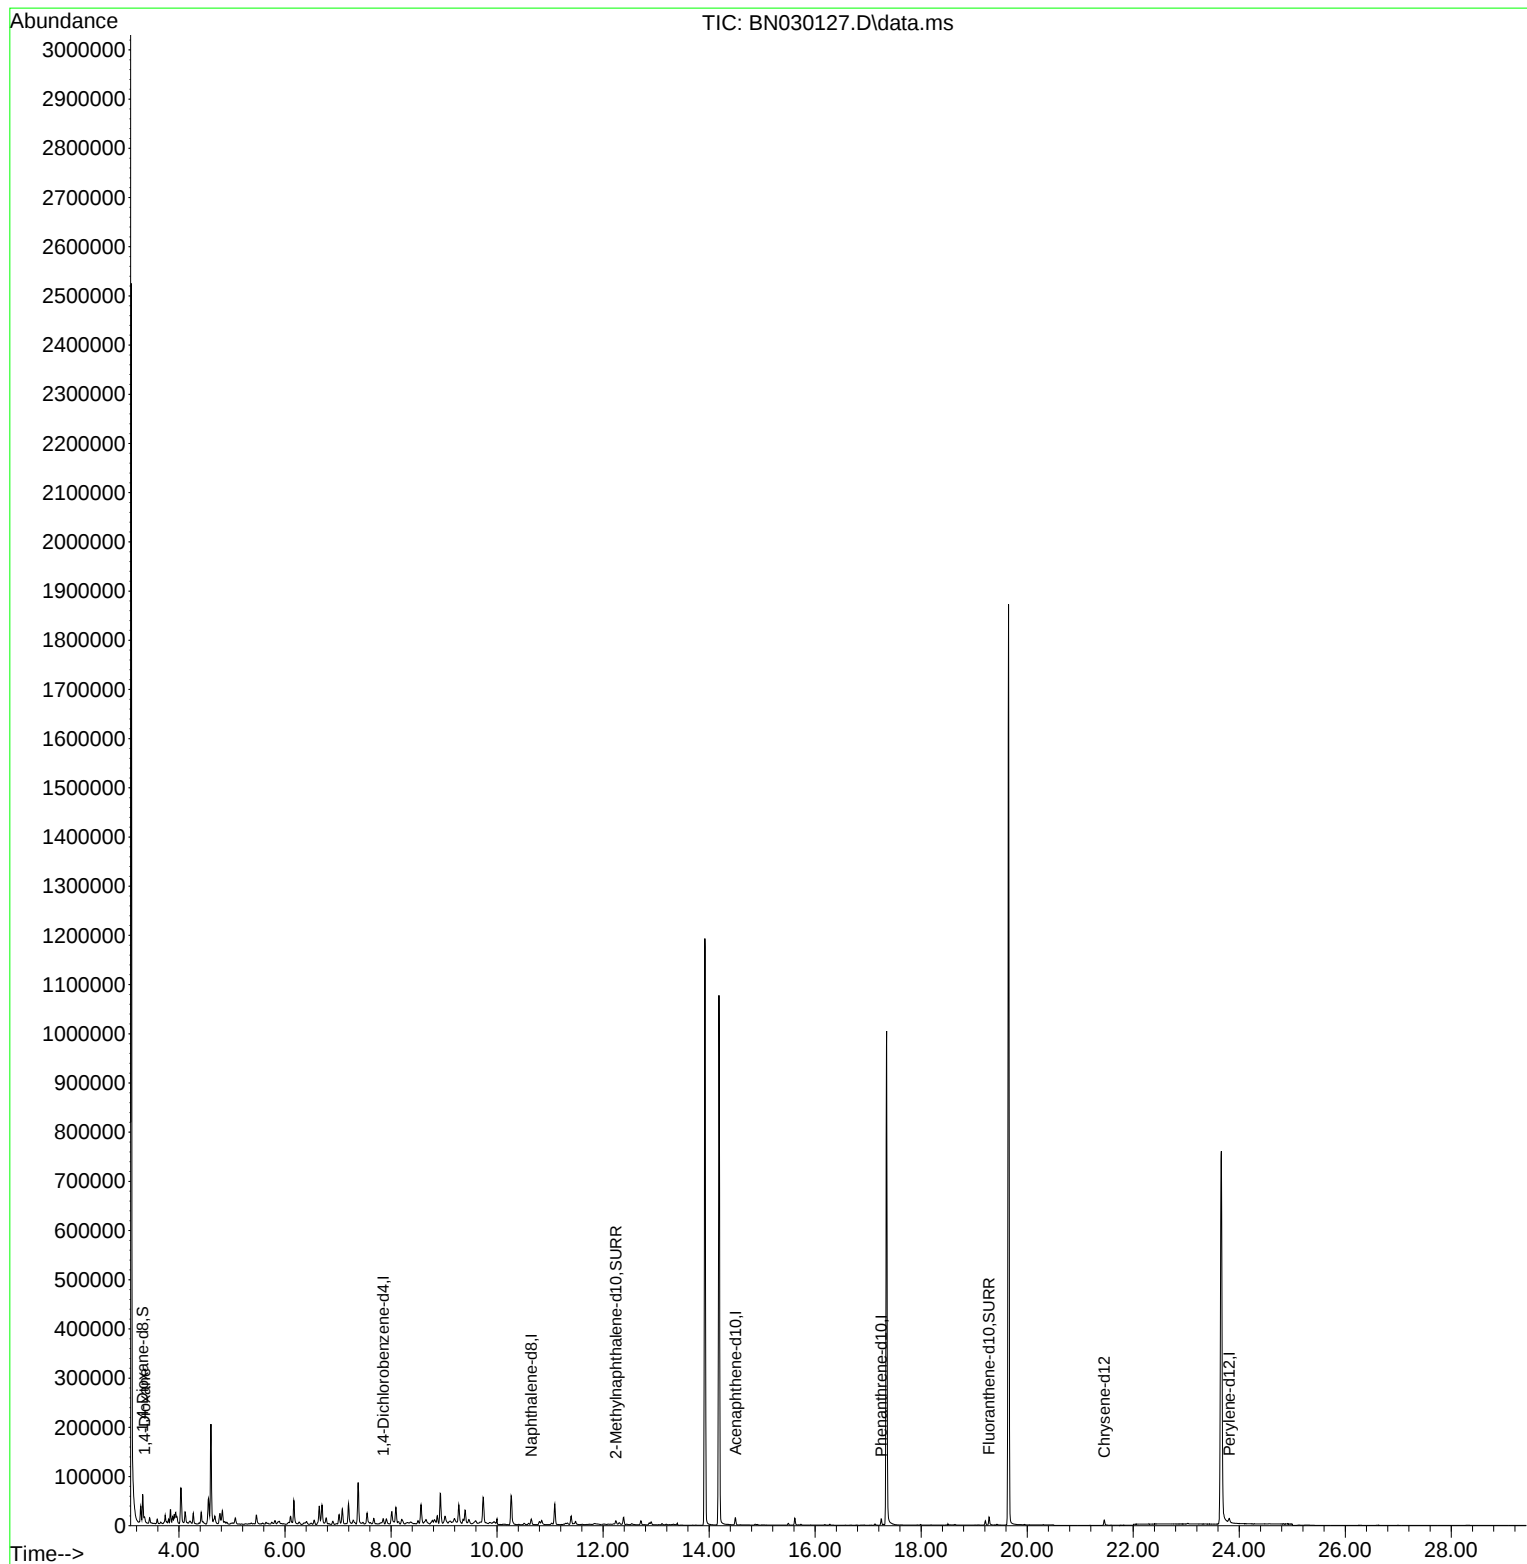

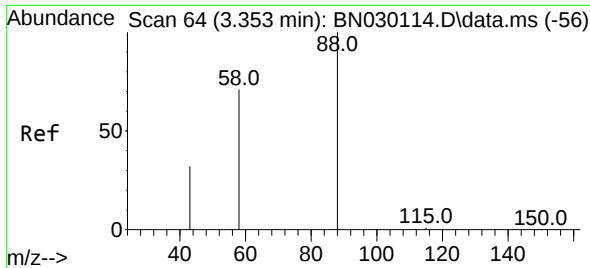

#2
 1,4-Dioxane
 Concen: 0.745 ng/ul
 RT: 3.353 min Scan# 64
 Delta R.T. 0.000 min
 Lab File: BN030127.D
 Acq: 28 Feb 2024 13:01

Instrument :
 BNA_N
 ClientSampleId :
 C0AB3

Tgt Ion: 88 Resp: 5807
 Ion Ratio Lower Upper
 88 100
 43 81.1 21.8 32.6#
 58 58.1 39.3 58.9

