

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
 Data File : BN030128.D
 Acq On : 28 Feb 2024 13:37
 Operator : MA/JU
 Sample : P1498-13
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD2

Manual Integrations
 APPROVED

Reviewed By :Jagrut
 Upadhyay

Quant Time: Feb 28 14:05:28 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 27 23:49:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.855	152	5008	0.400	ng/ul	0.00
4) Naphthalene-d8	10.645	136	15192	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.497	164	7592	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.247	188	14777	0.400	ng/ul	-0.02
17) Chrysene-d12	21.449	240	10424	0.400	ng/ul	-0.02
23) Perylene-d12	23.808	264	11959	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.311	96	52610m	8.425	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.240	152	9062	0.469	ng/ul	0.00
18) Fluoranthene-d10	19.281	212	16214	0.473	ng/ul	-0.01
Target Compounds						
2) 1,4-Dioxane	3.353	88	8740	1.286	ng/ul#	Qvalue 69

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
Data File : BN030128.D
Acq On : 28 Feb 2024 13:37
Operator : MA/JU
Sample : P1498-13
Misc :
ALS Vial : 33 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C0AD2

Manual Integrations
APPROVED

Reviewed By :Jagrut
Upadhyay


Quant Time: Feb 28 14:05:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 23:49:29 2024
Response via : Initial Calibration

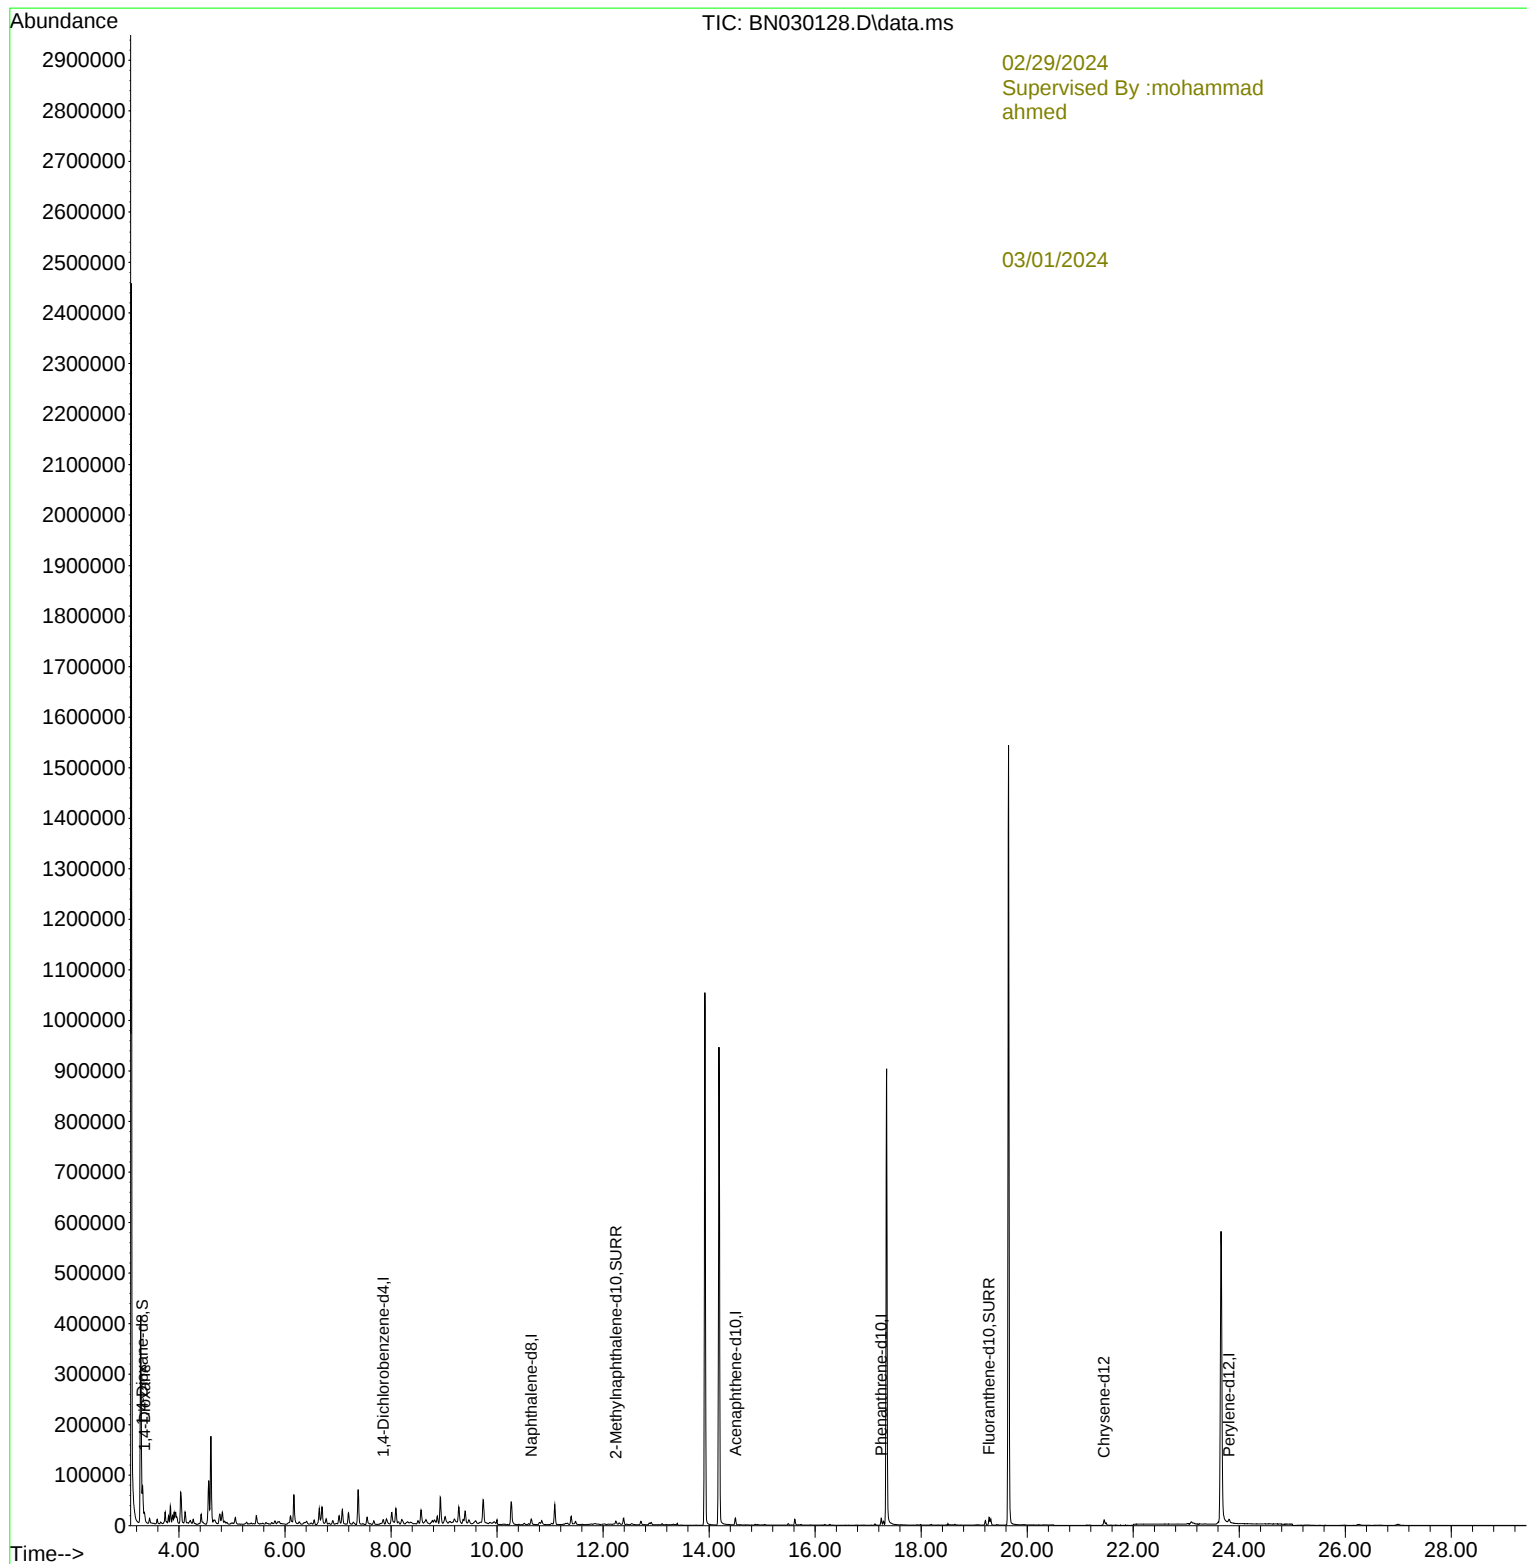

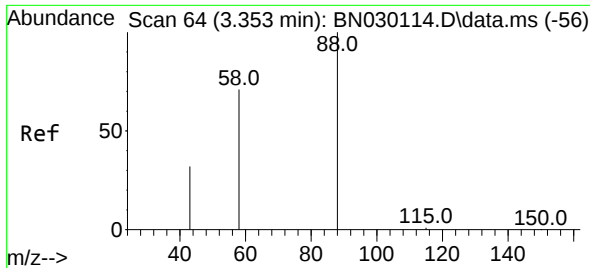

#2
 1,4-Dioxane
 Concen: 1.286 ng/ul
 RT: 3.353 min Scan# 64
 Delta R.T. 0.000 min
 Lab File: BN030128.D
 Acq: 28 Feb 2024 13:37



Instrument :
 BNA_N
 ClientSampleId :
 C0AD2

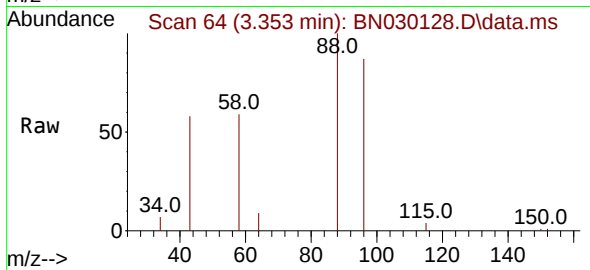

Tgt Ion: 88 Resp: 8740
 Ion Ratio Lower Upper
 88 100
 43 57.7 21.8 32.6
 58 59.3 39.3 58.9

Manual Integrations
 APPROVED

Reviewed By :Jagrut
 Upadhyay

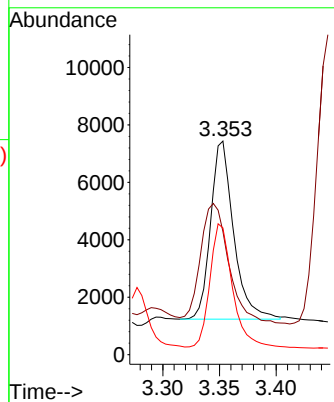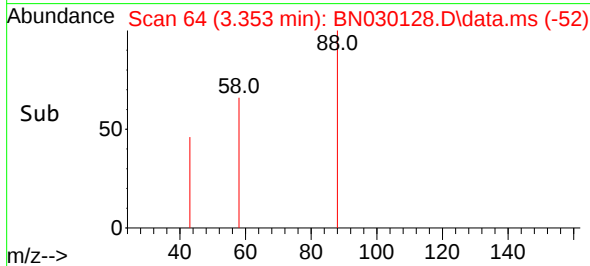

02/29/2024
 Supervised By :mohammad
 ahmed

03/01/2024