

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
 Data File : BN030145.D
 Acq On : 29 Feb 2024 00:26
 Operator : MA/JU
 Sample : P1494-20
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH3X7

Quant Time: Feb 29 02:04:09 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 27 23:49:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.863	152	5394	0.400	ng/ul	0.00
4) Naphthalene-d8	10.656	136	16082	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.506	164	8116	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.255	188	11271	0.400	ng/ul	0.00
17) Chrysene-d12	21.458	240	7144	0.400	ng/ul	0.00
23) Perylene-d12	23.817	264	8421	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.319	96	28827	4.286	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.251	152	10110	0.494	ng/ul	0.00
18) Fluoranthene-d10	19.290	212	14877	0.634	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.349	88	700	0.096	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
Data File : BN030145.D
Acq On : 29 Feb 2024 00:26
Operator : MA/JU
Sample : P1494-20
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3X7

Quant Time: Feb 29 02:04:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 23:49:29 2024
Response via : Initial Calibration

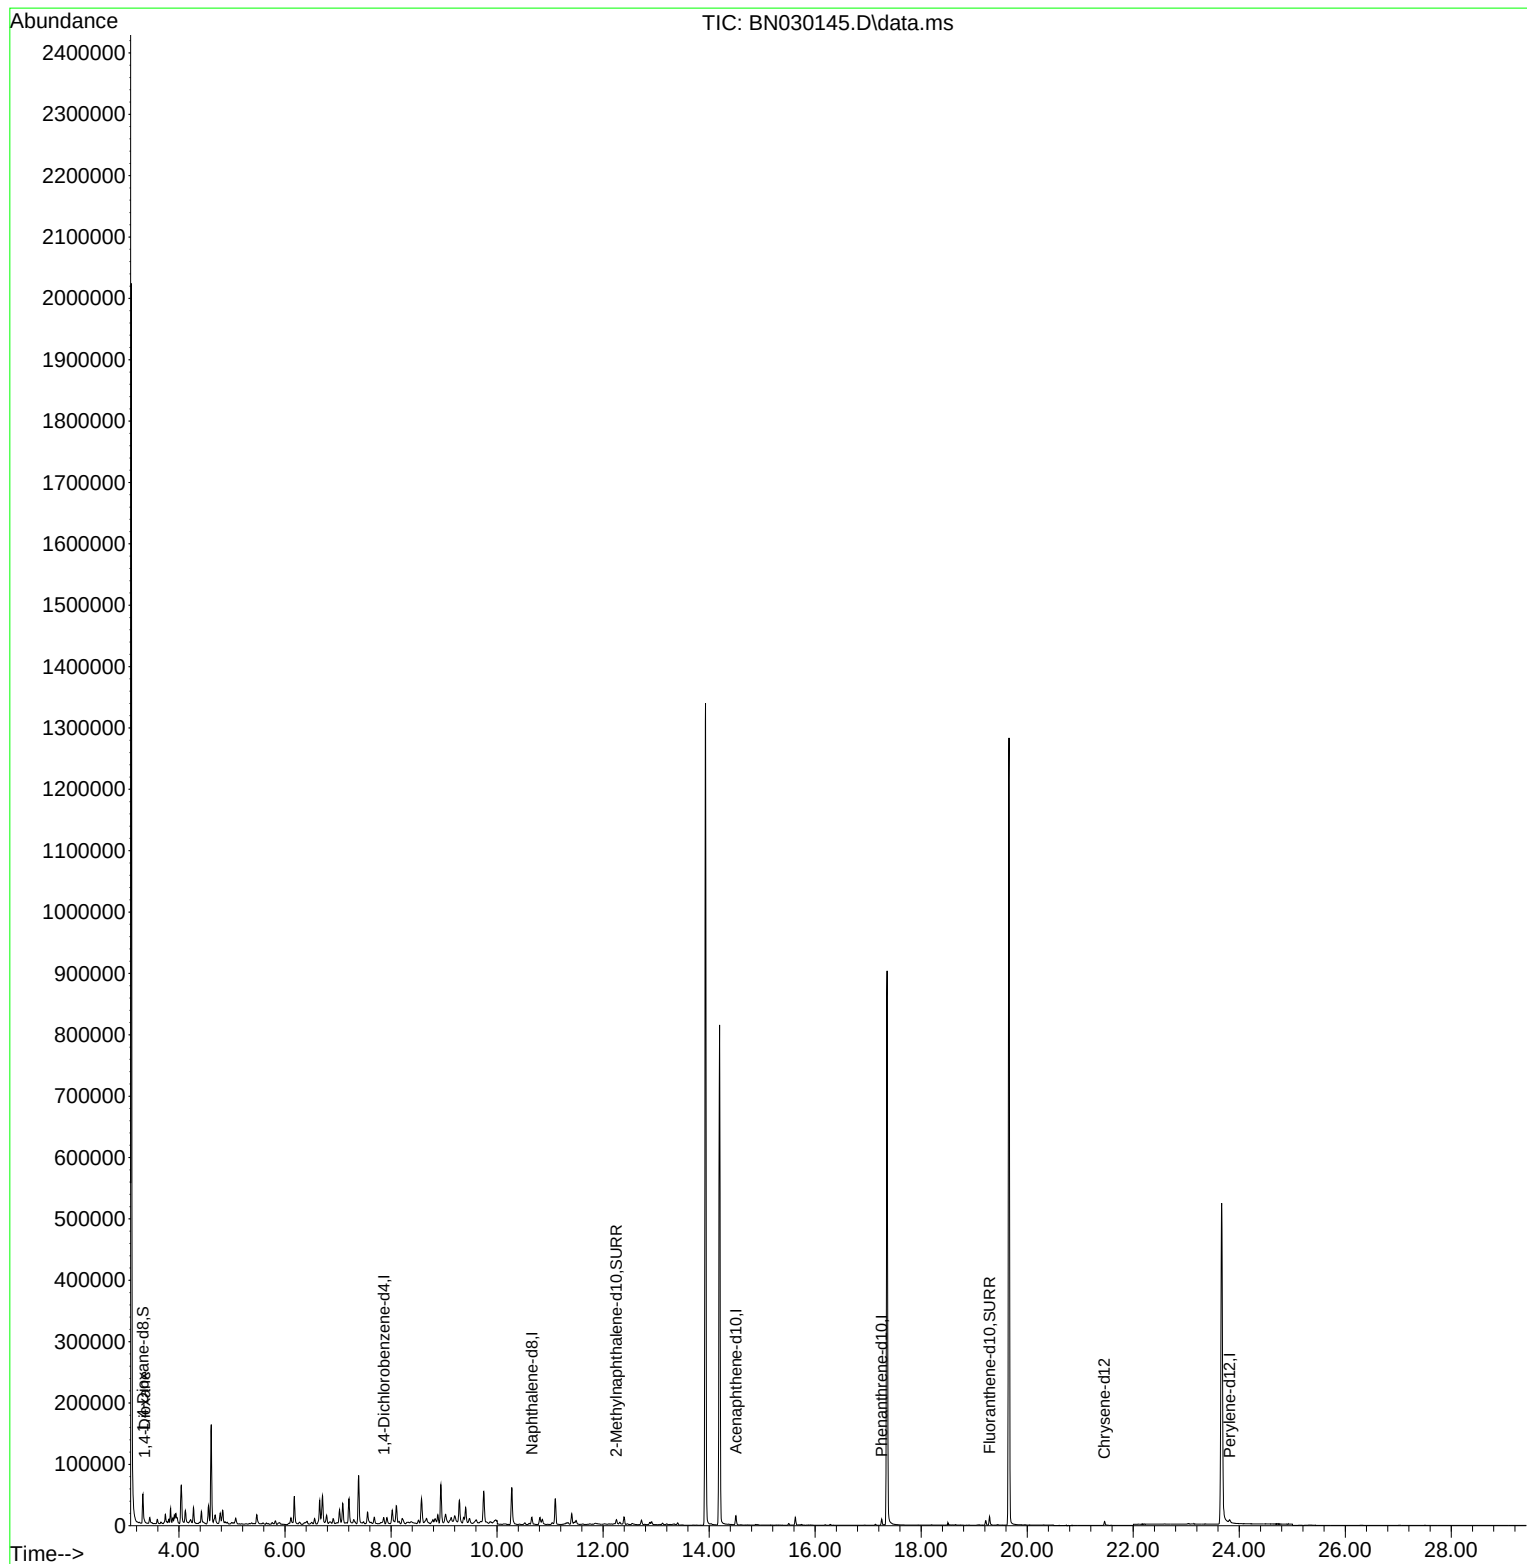

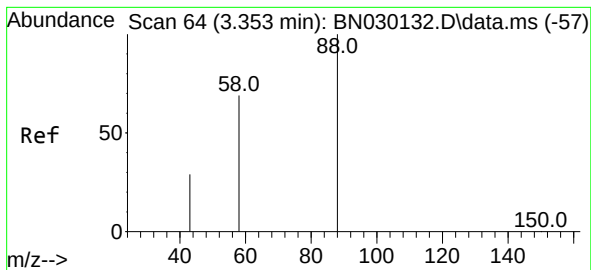

#2

1,4-Dioxane

Concen: 0.096 ng/ul

RT: 3.349 min Scan# 61

Delta R.T. -0.004 min

Lab File: BN030145.D


Acq: 29 Feb 2024 00:26

Instrument :

BNA_N

ClientSampleId :

BH3X7

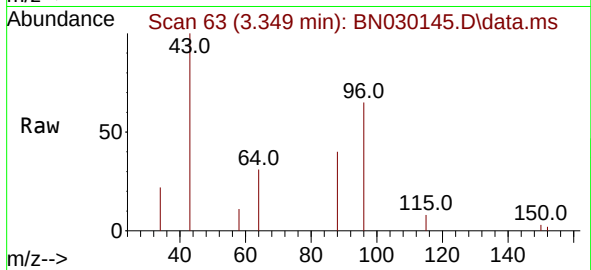

Tgt Ion: 88 Resp: 700

Ion Ratio Lower Upper

88 100

43 251.3 21.8 32.6#

58 27.5 39.3 58.9#

