

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
 Data File : BN030162.D
 Acq On : 29 Feb 2024 11:14
 Operator : MA/JU
 Sample : P1535-02
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC6

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 02/29/2024
 Supervised By :mohammad ahmed 03/01/2024

Quant Time: Feb 29 11:51:06 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 27 23:49:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.922	152	4045	0.400	ng/ul	0.07
4) Naphthalene-d8	10.722	136	6669	0.400	ng/ul	0.07
9) Acenaphthene-d10	14.562	164	3682	0.400	ng/ul	# 0.07
13) Phenanthrene-d10	17.310	188	10018m	0.400	ng/ul	0.05
17) Chrysene-d12	21.508	240	6338	0.400	ng/ul	0.04
23) Perylene-d12	23.905	264	5847	0.400	ng/ul	0.08
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.345	96	21644	4.291	ng/ul	0.03
6) 2-Methylnaphthalene-d10	12.322	152	3932	0.463	ng/ul	0.08
18) Fluoranthene-d10	19.341	212	12918	0.620	ng/ul	0.05
Target Compounds						Qvalue
2) 1,4-Dioxane	3.382	88	4448	0.810	ng/ul	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
Data File : BN030162.D
Acq On : 29 Feb 2024 11:14
Operator : MA/JU
Sample : P1535-02
Misc :
ALS Vial : 69 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C0AC6

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 02/29/2024
Supervised By :mohammad ahmed 03/01/2024


Quant Time: Feb 29 11:51:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 23:49:29 2024
Response via : Initial Calibration

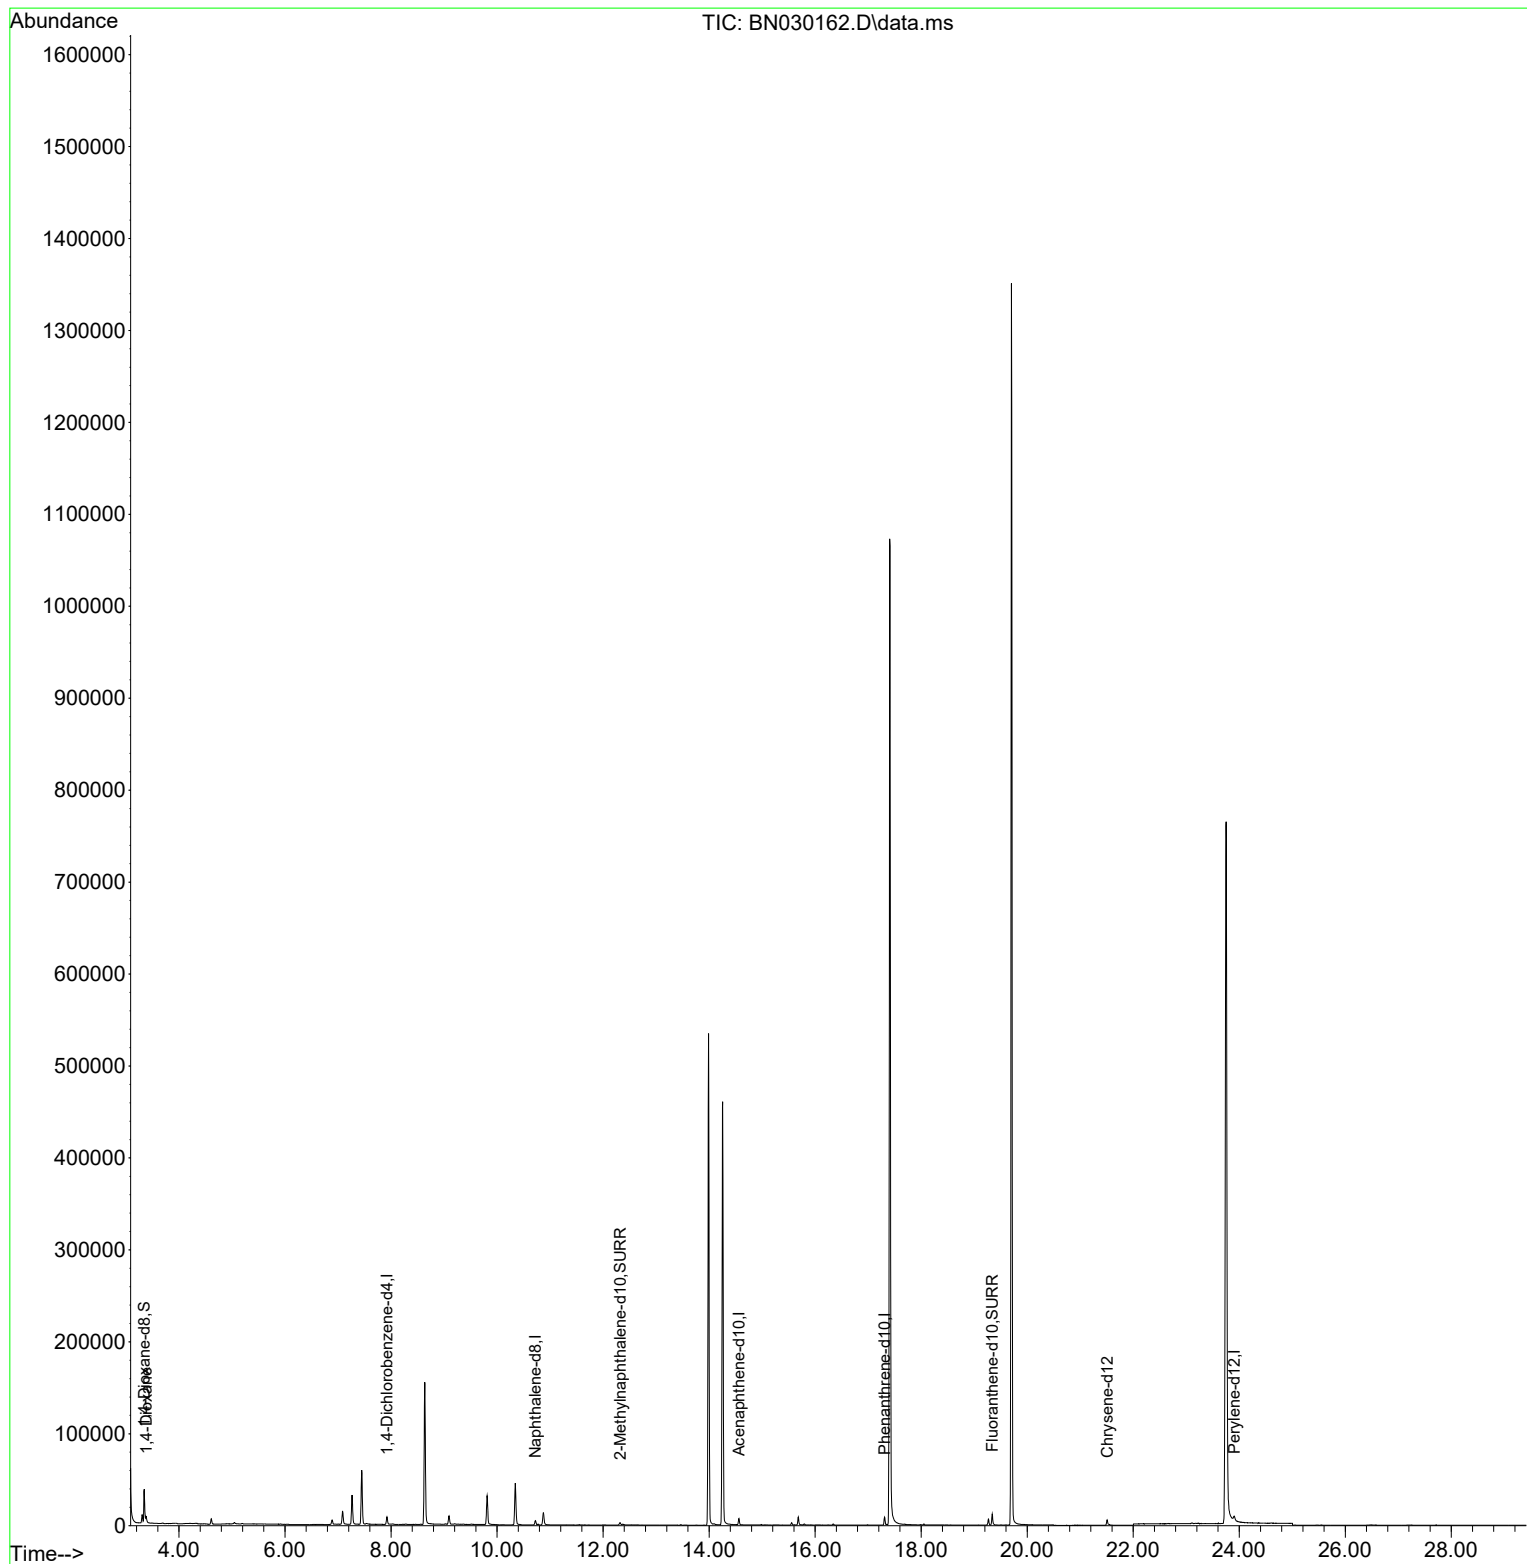

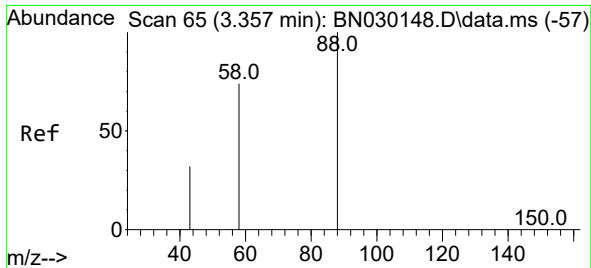

#2
 1,4-Dioxane
 Concen: 0.810 ng/ul
 RT: 3.382 min Scan# 71
 Delta R.T. 0.030 min
 Lab File: BN030162.D
 Acq: 29 Feb 2024 11:14

Instrument :
 BNA_N
 ClientSampleId :
 C0AC6

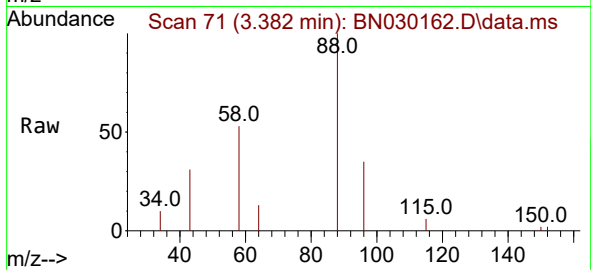

Tgt Ion: 88 Resp: 4448
 Ion Ratio Lower Upper
 88 100
 43 30.8 21.8 32.6
 58 53.0 39.3 58.9

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 02/29/2024
 Supervised By :mohammad ahmed 03/01/2024

