

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
 Data File : BN030164.D
 Acq On : 29 Feb 2024 12:26
 Operator : MA/JU
 Sample : P1501-23
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E10C2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/01/2024
 Supervised By :mohammad ahmed 03/01/2024

Quant Time: Feb 29 13:25:32 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 27 23:49:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.998	152	2572	0.400	ng/ul	0.14
4) Naphthalene-d8	10.804	136	7975	0.400	ng/ul	0.15
9) Acenaphthene-d10	14.631	164	4797m	0.400	ng/ul	0.13
13) Phenanthrene-d10	17.373	188	10591m	0.400	ng/ul	0.11
17) Chrysene-d12	21.565	240	8258m	0.400	ng/ul	0.10
23) Perylene-d12	24.000	264	5418m	0.400	ng/ul	0.17
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.374	96	15431	4.812	ng/ul	0.06
6) 2-Methylnaphthalene-d10	12.399	152	4998	0.493	ng/ul	0.15
18) Fluoranthene-d10	19.402	212	15547m	0.573	ng/ul	0.11
Target Compounds						Qvalue
5) Naphthalene	10.854	128	592	0.026	ng/ul#	67

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
Data File : BN030164.D
Acq On : 29 Feb 2024 12:26
Operator : MA/JU
Sample : P1501-23
Misc :
ALS Vial : 71 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
E10C2

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/01/2024
Supervised By :mohammad ahmed 03/01/2024

Quant Time: Feb 29 13:25:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 23:49:29 2024
Response via : Initial Calibration

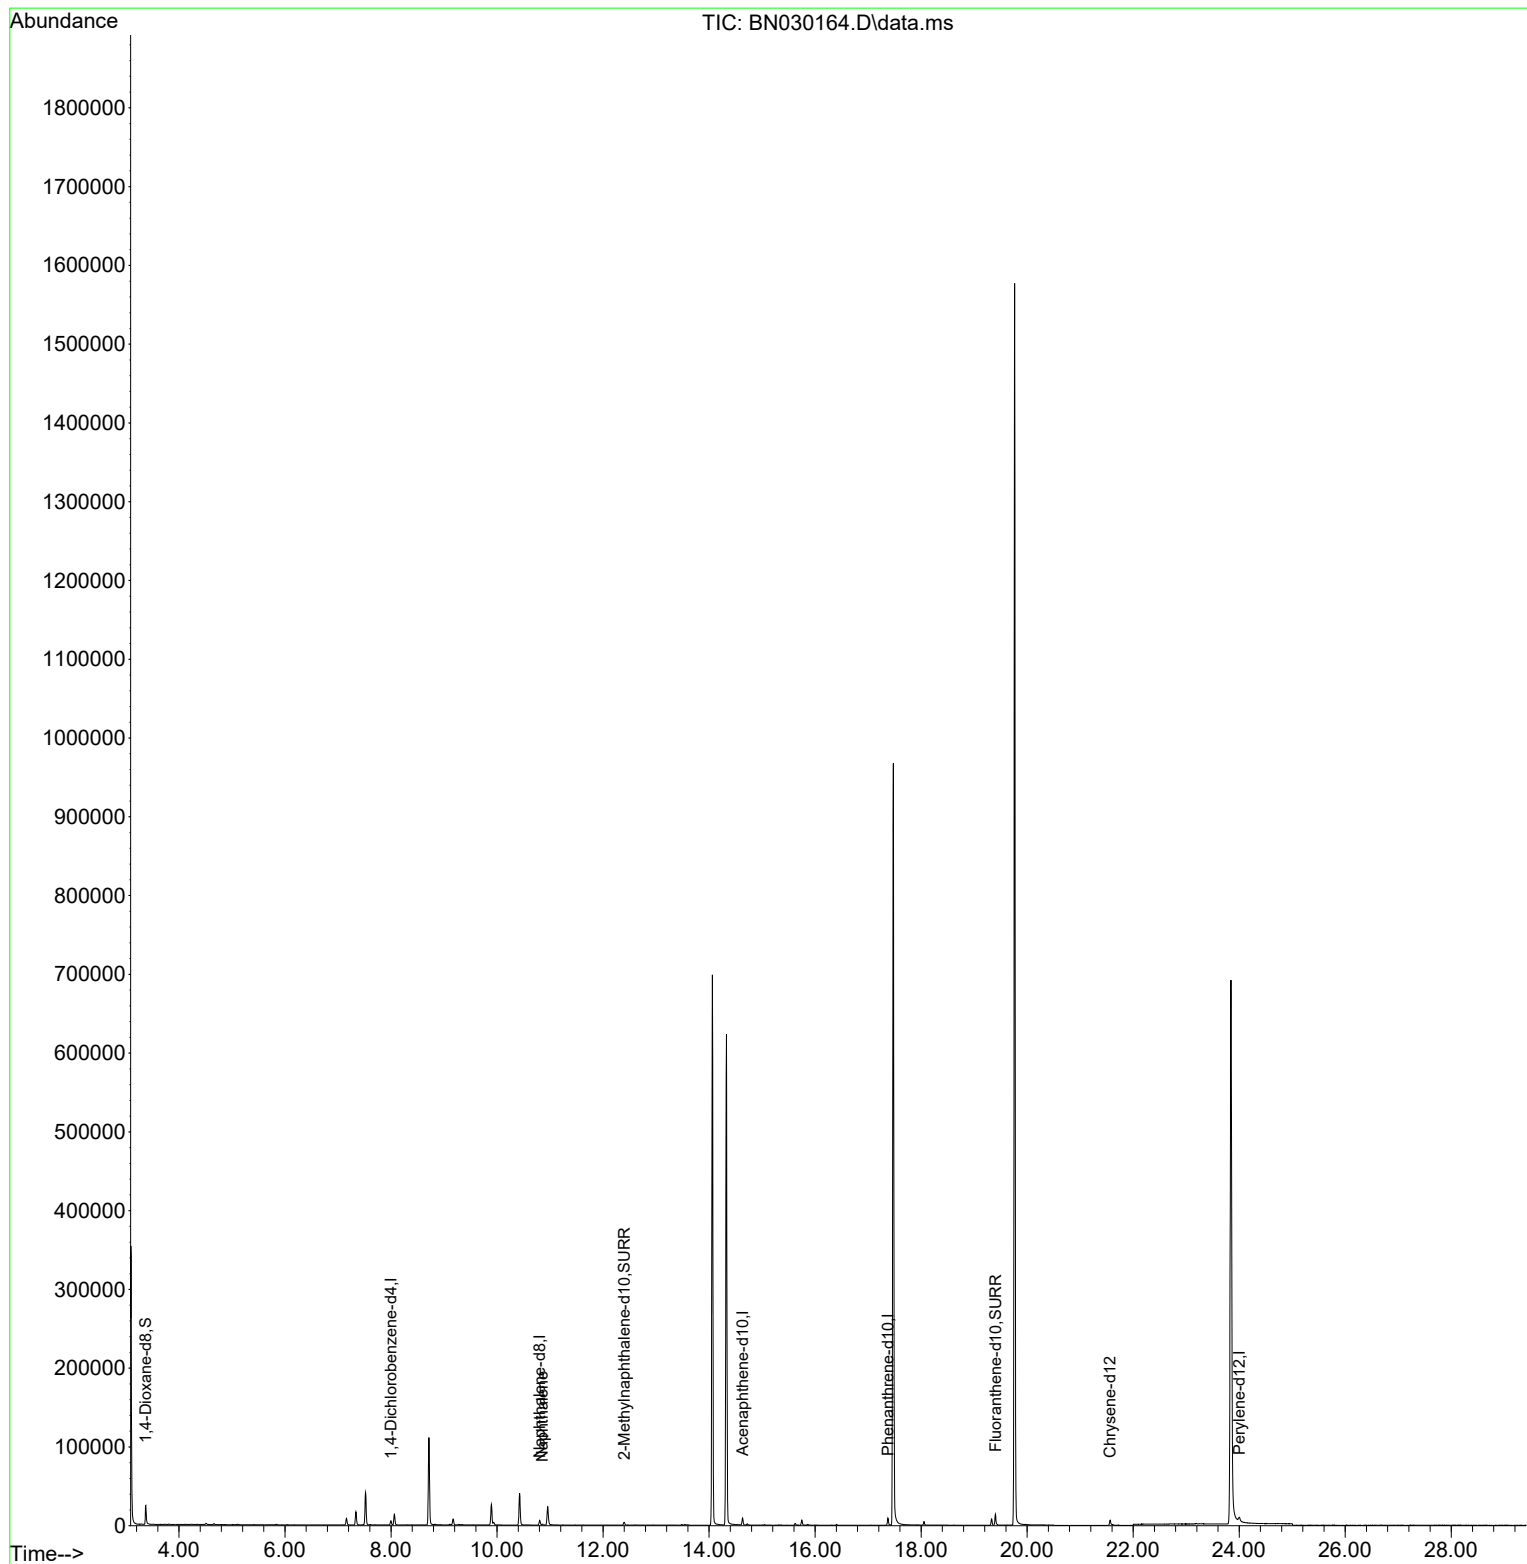

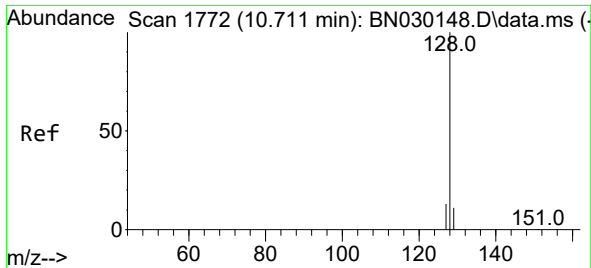

#5

Naphthalene

Concen: 0.026 ng/ul

RT: 10.854 min Scan# 11

Delta R.T. 0.154 min

Lab File: BN030164.D


Acq: 29 Feb 2024 12:26

Instrument :

BNA_N

ClientSampleId :

E10C2

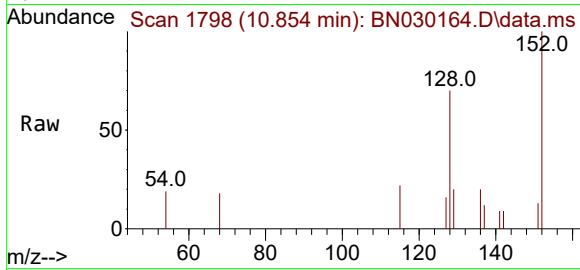

Tgt Ion:128 Resp: 592

Ion Ratio Lower Upper

128 100

129 28.4 9.1 13.7

127 23.6 11.0 16.6

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 03/01/2024

Supervised By :mohammad ahmed 03/01/2024

