
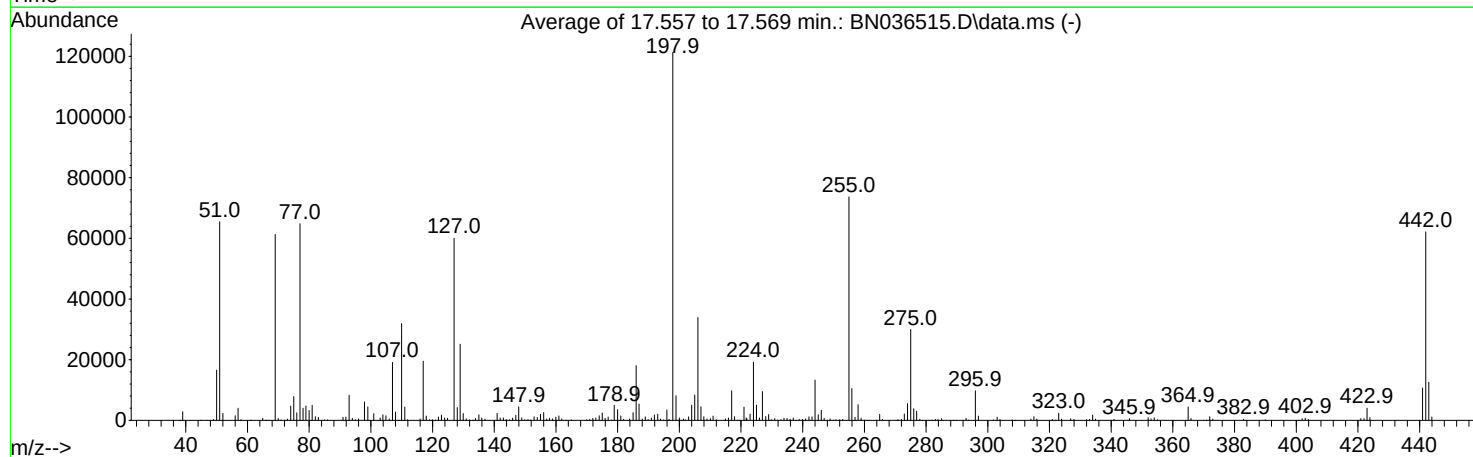


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022825\
Data File : BN036515.D
Acq On : 28 Feb 2025 12:21
Operator : RC/JU
Sample : DFTPP267
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP370

Integration File: LSCINT.P

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN022825.MA.M
Title : SVOA CALIBRATION
Last Update : Mon Mar 03 12:45:15 2025

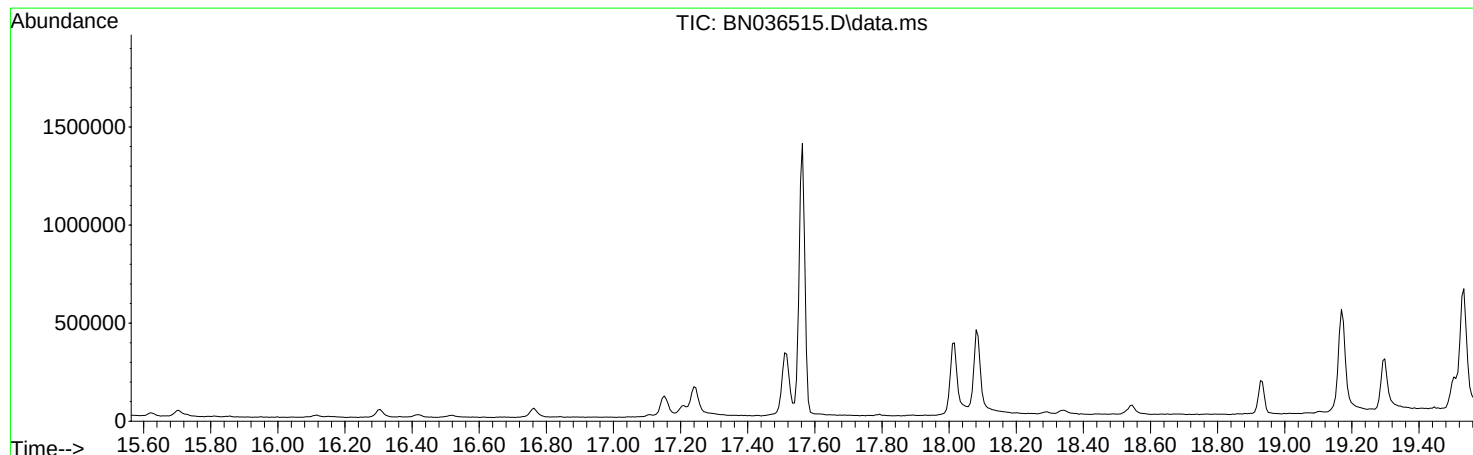

AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2454

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	54.0	65470	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	50.5	61288	PASS
70	69	0.00	2	1.0	643	PASS
127	198	10	80	49.5	60003	PASS
197	198	0.00	2	0.3	331	PASS
198	198	100	100	100.0	121256	PASS
199	198	5	9	6.7	8104	PASS
275	198	10	60	24.7	29979	PASS
365	198	1	100	3.7	4440	PASS
441	198	0.01	100	8.8	10666	PASS
442	198	50	100	51.2	62133	PASS
443	442	15	24	20.2	12576	PASS