


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA N\Data\BN030118\
 Data File : BN000206.D
 Acq On : 01 Mar 2018 08:10
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_N\METHODS\8270-SIM-BN022718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 27 15:07:57 2018

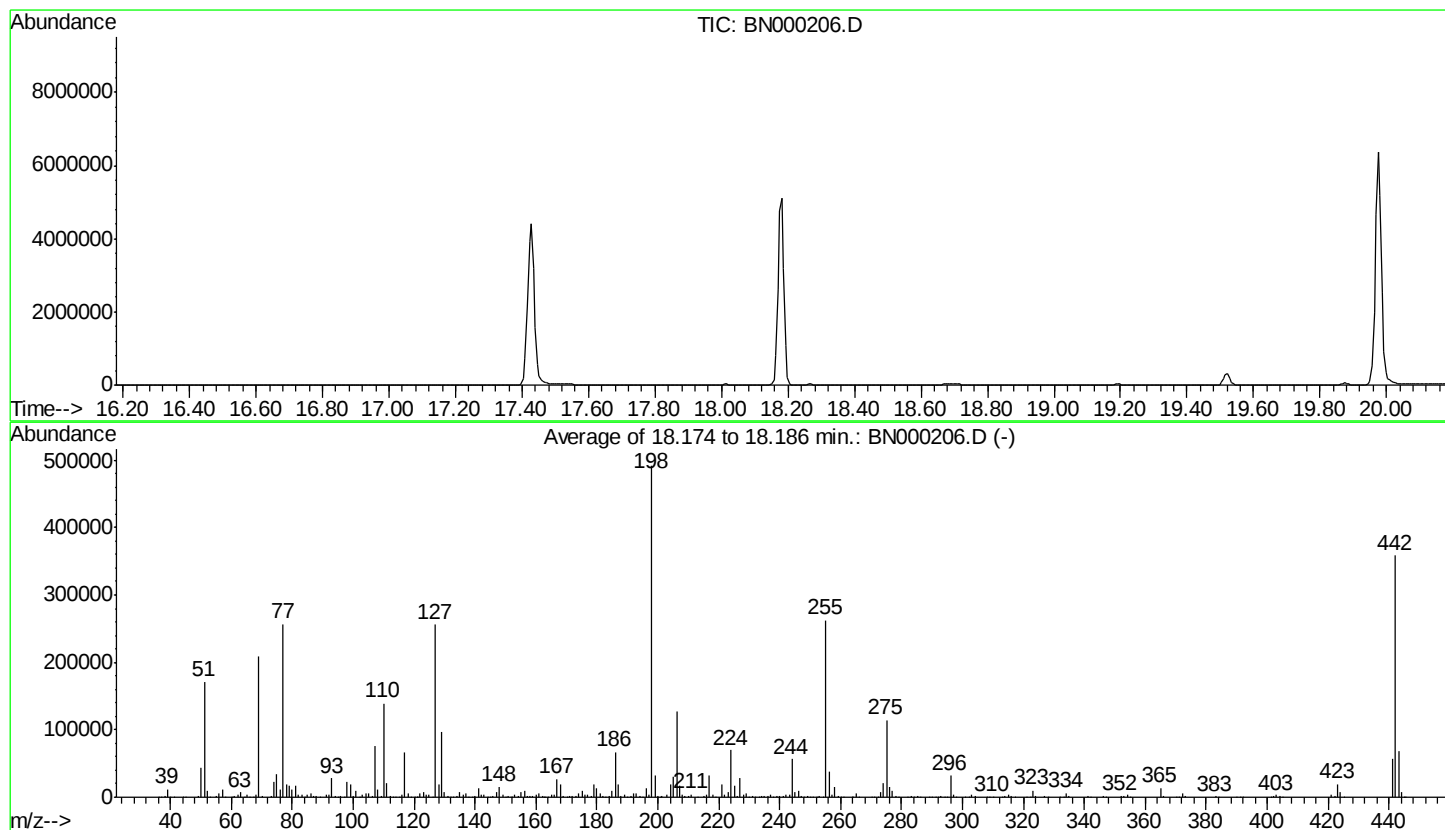

AutoFind: Scans 2582, 2583, 2584; Background Corrected with Scan 2575

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.8	171045	PASS
68	69	0.00	2	1.9	3958	PASS
69	198	0.00	100	42.5	208768	PASS
70	69	0.00	2	0.5	1123	PASS
127	198	10	80	52.0	255616	PASS
197	198	0.00	2	0.7	3432	PASS
198	198	100	100	100.0	491669	PASS
199	198	5	9	6.7	32989	PASS
275	198	10	60	23.3	114477	PASS
365	198	1	100	2.9	14086	PASS
441	443	0.01	100	83.4	57474	PASS
442	198	50	100	72.9	358421	PASS
443	442	15	24	19.2	68888	PASS