


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA N\Data\BN030118\
 Data File : BN000215.D
 Acq On : 01 Mar 2018 13:53
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_N\METHODS\8270-SIM-BN022718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 27 15:07:57 2018

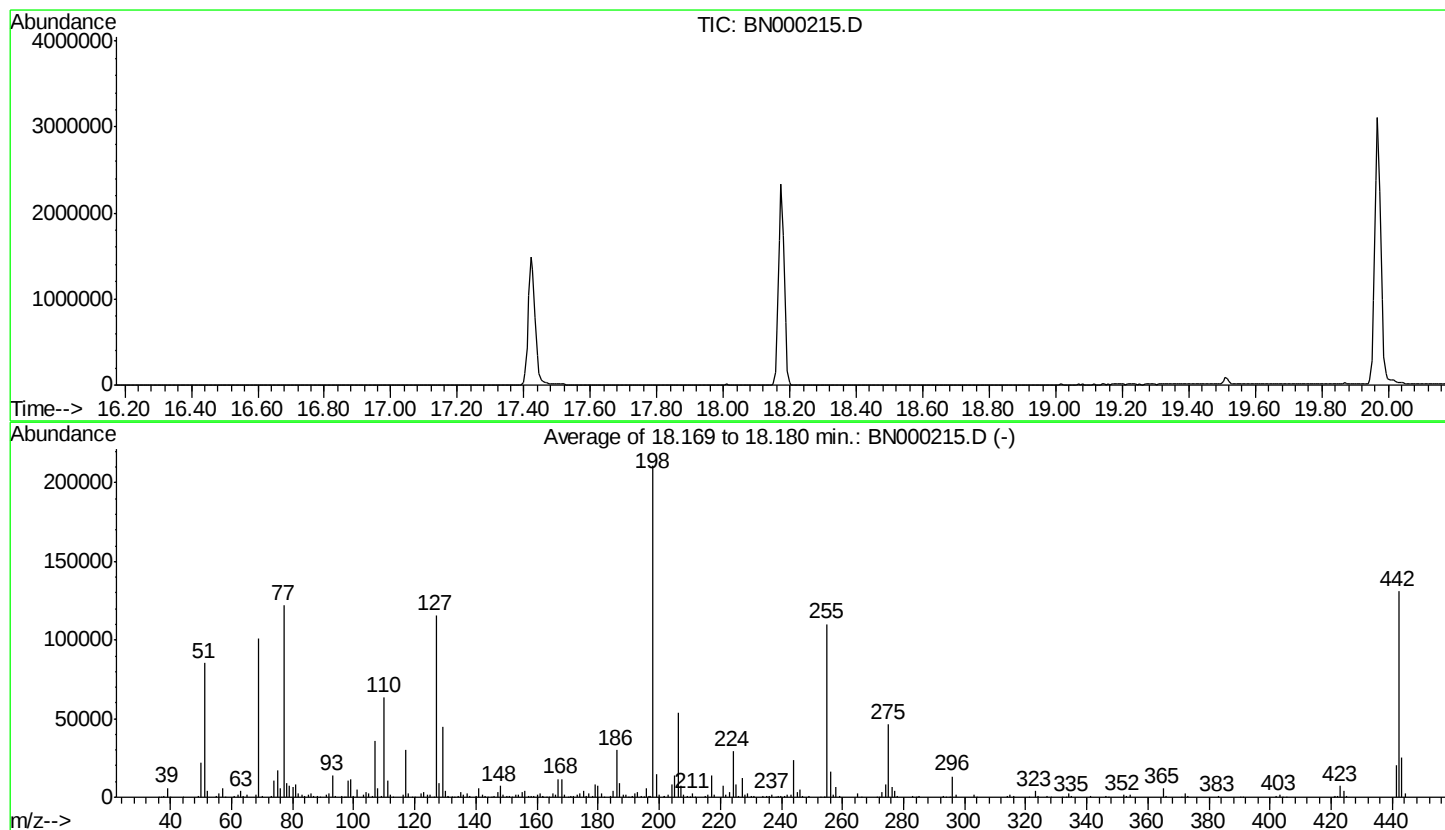

AutoFind: Scans 2581, 2582, 2583; Background Corrected with Scan 2575

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.4	85237	PASS
68	69	0.00	2	1.7	1741	PASS
69	198	0.00	100	48.0	101274	PASS
70	69	0.00	2	0.6	626	PASS
127	198	10	80	54.7	115490	PASS
197	198	0.00	2	0.4	941	PASS
198	198	100	100	100.0	210944	PASS
199	198	5	9	7.0	14822	PASS
275	198	10	60	21.9	46141	PASS
365	198	1	100	2.6	5527	PASS
441	443	0.01	100	81.4	20484	PASS
442	198	50	100	62.1	131048	PASS
443	442	15	24	19.2	25150	PASS