
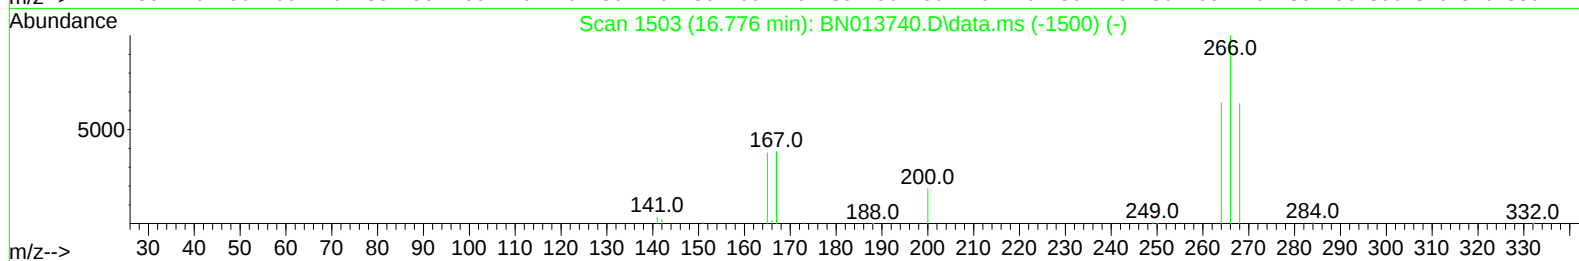
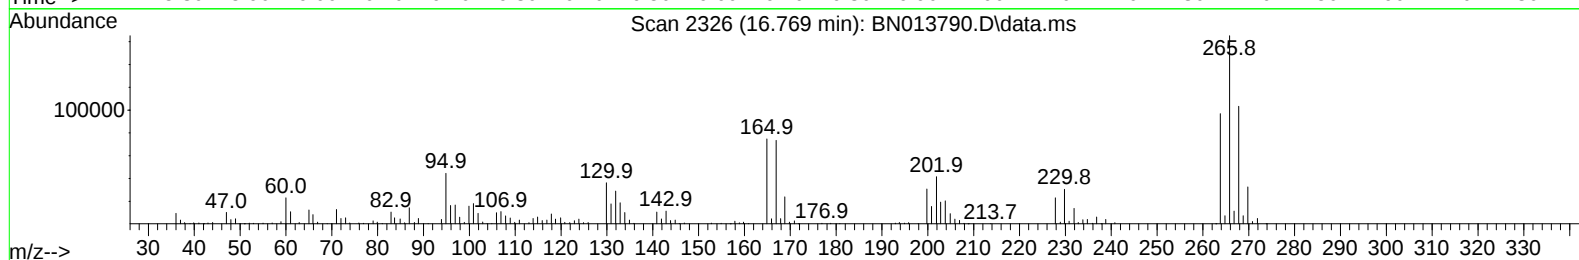


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030121\
 Data File : BN013790.D
 Acq On : 01 Mar 2021 11:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 01 11:55:38 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN022421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 25 11:31:11 2021
 Response via : Initial Calibration

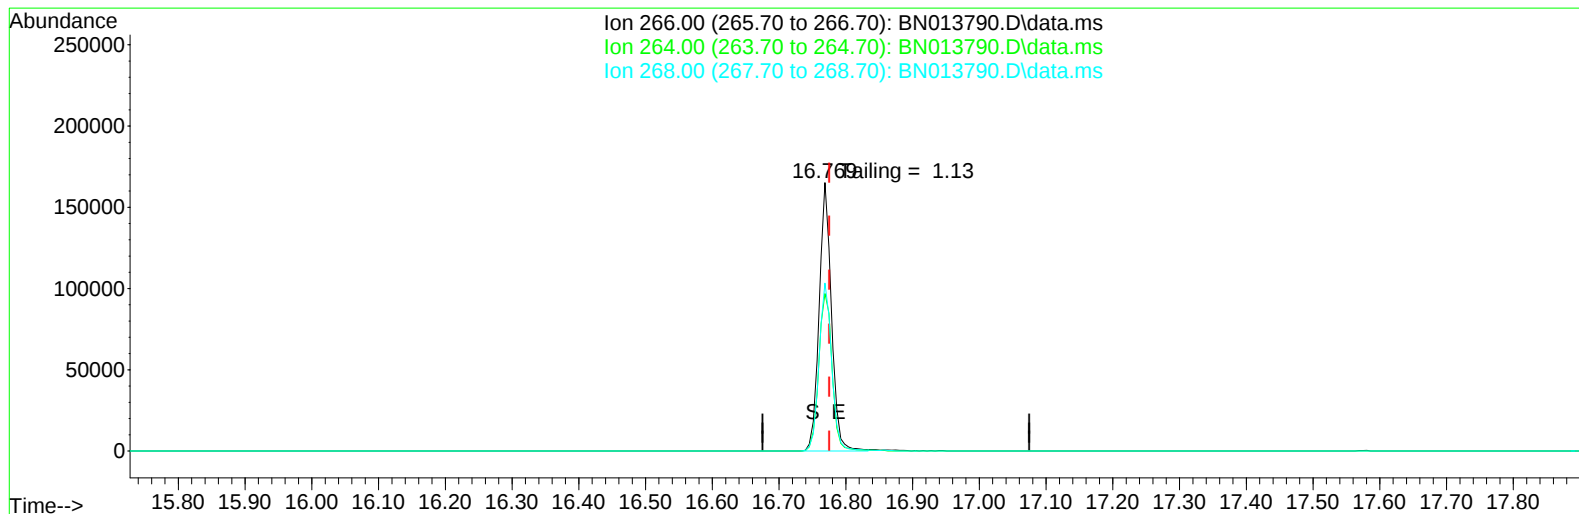

TIC: BN013790.D\data.ms

(24) Pentachlorophenol

16.769min (-0.006) 0.00 ng

response 212993

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	64.50	63.04
268.00	68.30	64.09
0.00	0.00	0.00