
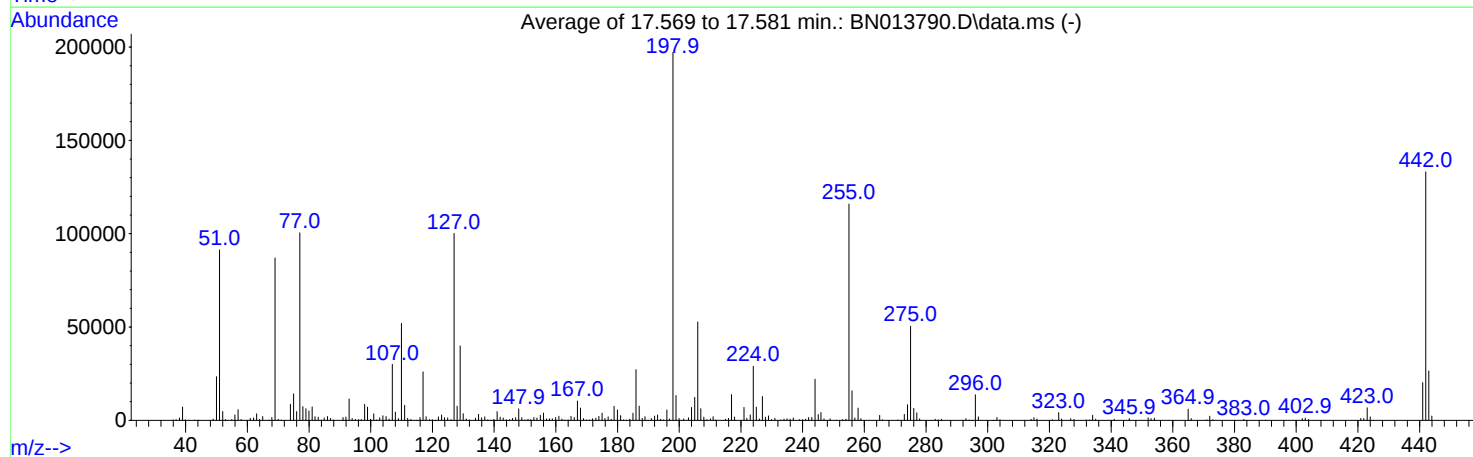


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030121\
 Data File : BN013790.D
 Acq On : 01 Mar 2021 11:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN022421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Feb 25 11:31:11 2021

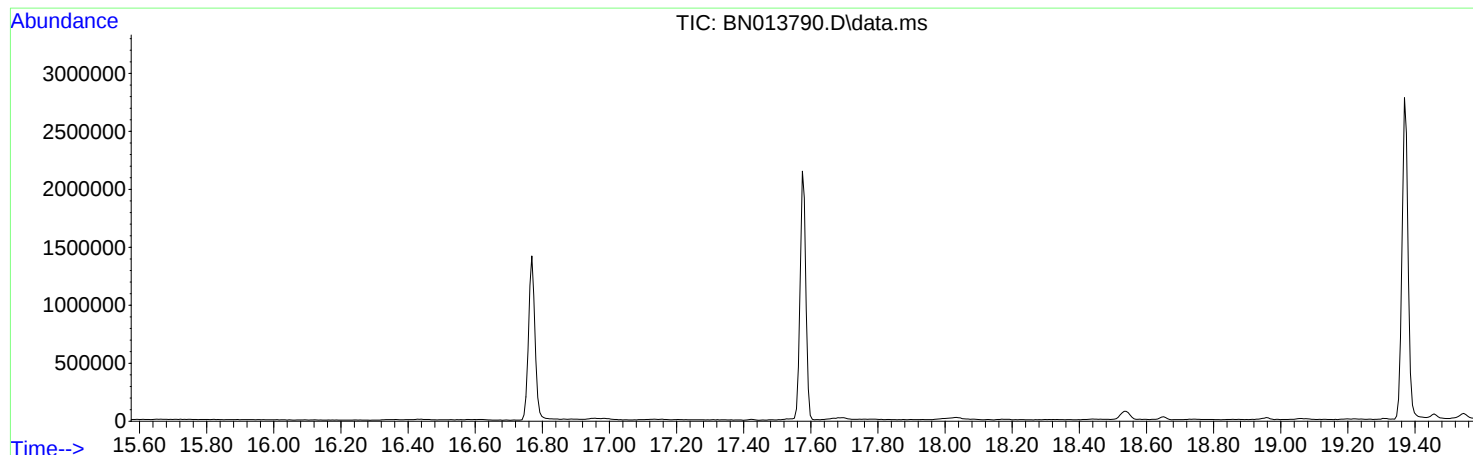




AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.3	91259	PASS
68	69	0.00	2	1.7	1507	PASS
69	198	0.00	100	44.2	87019	PASS
70	69	0.00	2	0.7	602	PASS
127	198	10	80	50.8	100128	PASS
197	198	0.00	2	0.4	799	PASS
198	198	100	100	100.0	197077	PASS
199	198	5	9	6.8	13381	PASS
275	198	10	60	25.6	50400	PASS
365	198	1	100	3.1	6030	PASS
441	198	0.01	100	10.2	20198	PASS
442	442	50	100	100.0	133152	PASS
443	442	15	24	19.9	26496	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030121\
Data File : BN013790.D
Acq On : 01 Mar 2021 11:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 02 00:02:32 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 26 07:31:37 2021
Response via : Initial Calibration

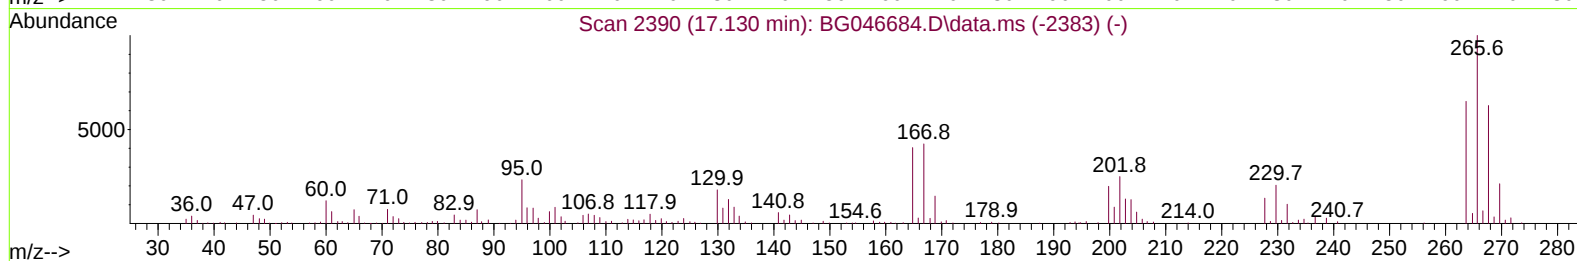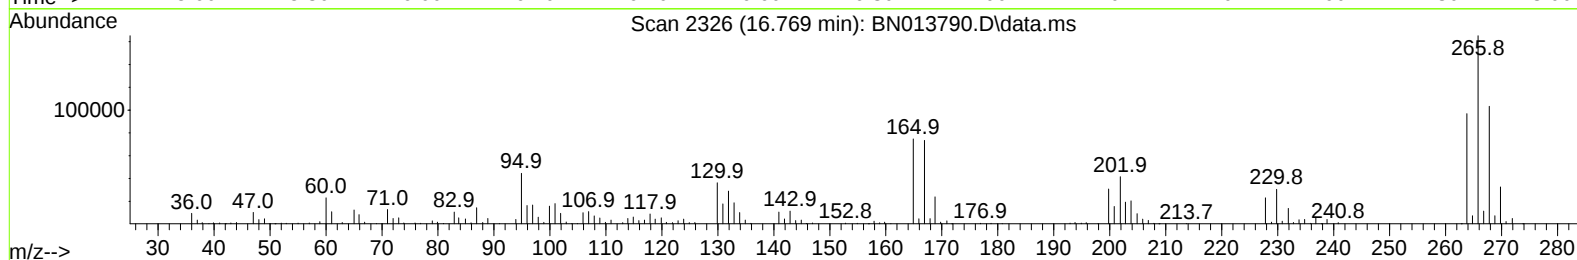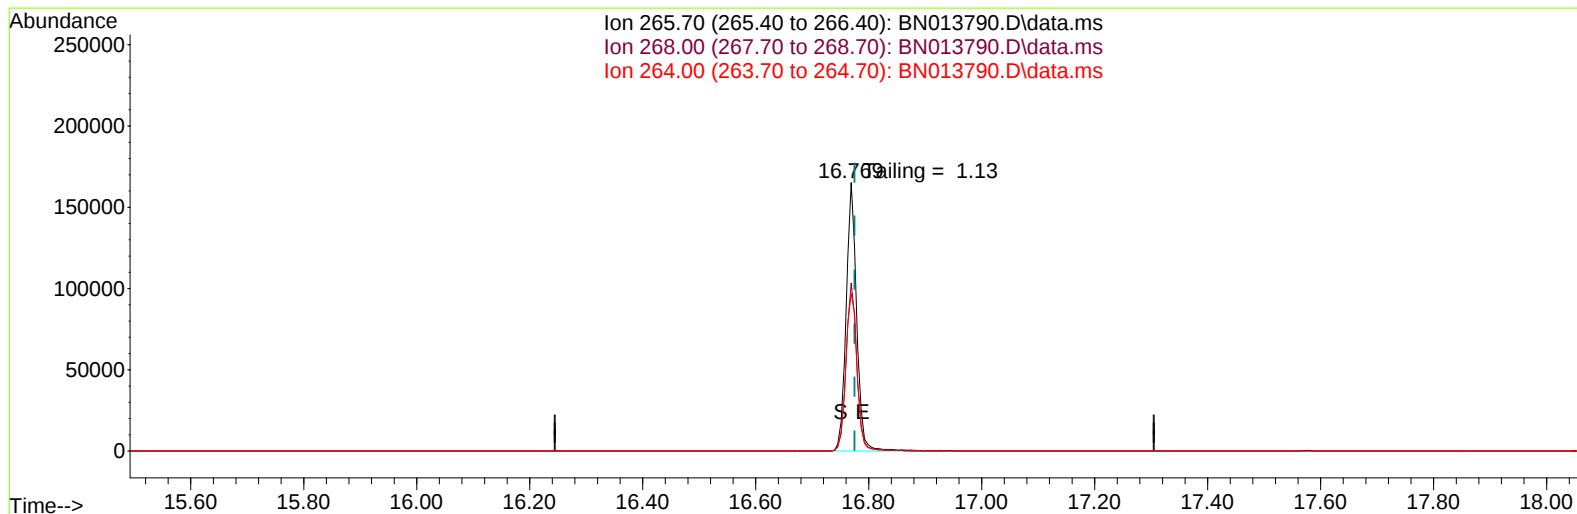

TIC: BN013790.D\data.ms

(70) Pentachlorophenol (C)

16.769min (-0.006) 22083.52 ng




response 212993

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.57
264.00	61.60	58.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030121\
 Data File : BN013790.D
 Acq On : 01 Mar 2021 11:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Mar 02 00:02:32 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 26 07:31:37 2021
 Response via : Initial Calibration

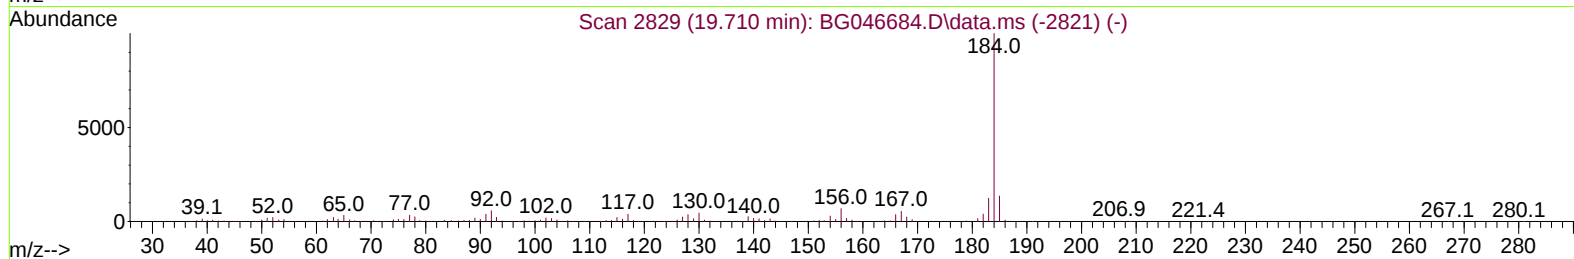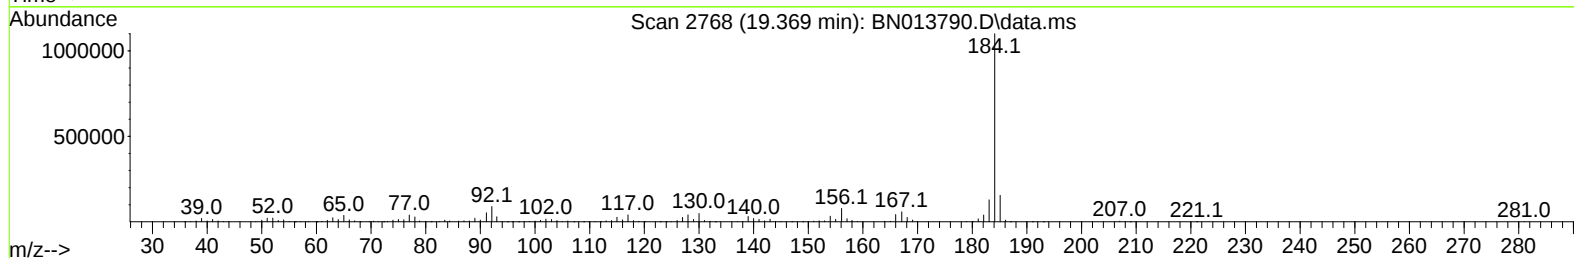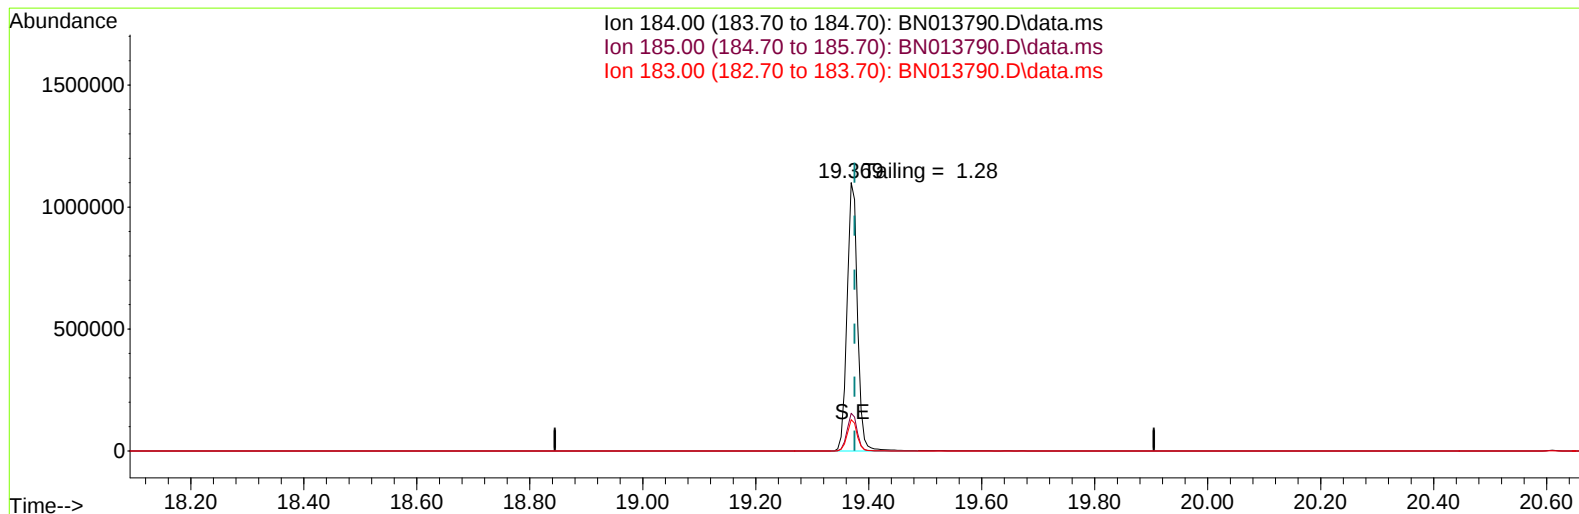

TIC: BN013790.D\data.ms

(77) Benzidine

19.369min (-0.006) 51307.57 ng

response 1402857

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.06
183.00	13.20	11.72
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_N
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
3/1/2021	BNA_N	<u>BN013790.D</u>
Compound Name	Response	Retention Time
DDT	672871	20.61
DDD	6985	20.16
DDE	912	19.66
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7897	680768	1.16

Instrument :
BNA_N
ClientSampleId :
DFTPP