
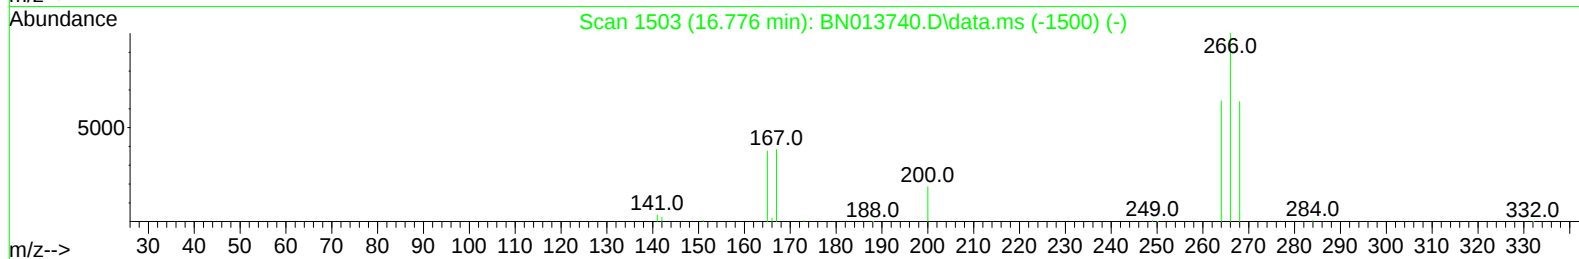
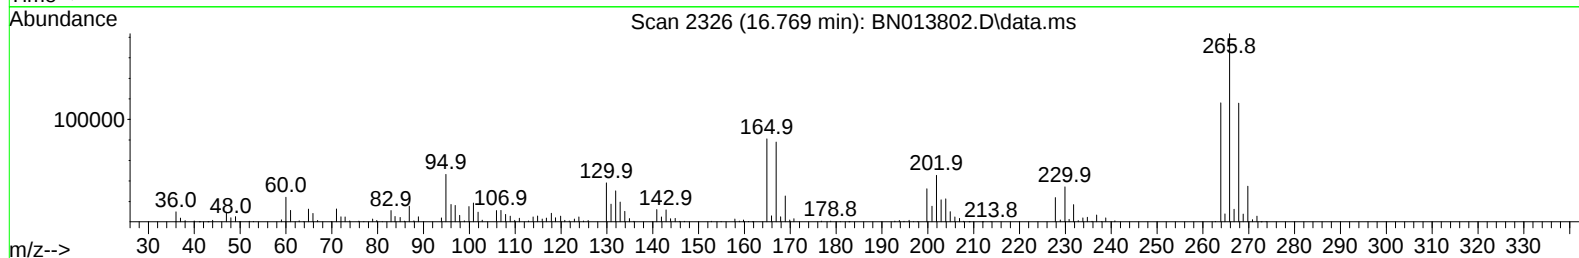


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030221\
Data File : BN013802.D
Acq On : 02 Mar 2021 09:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 02 10:15:53 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN022421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 25 11:31:11 2021
Response via : Initial Calibration

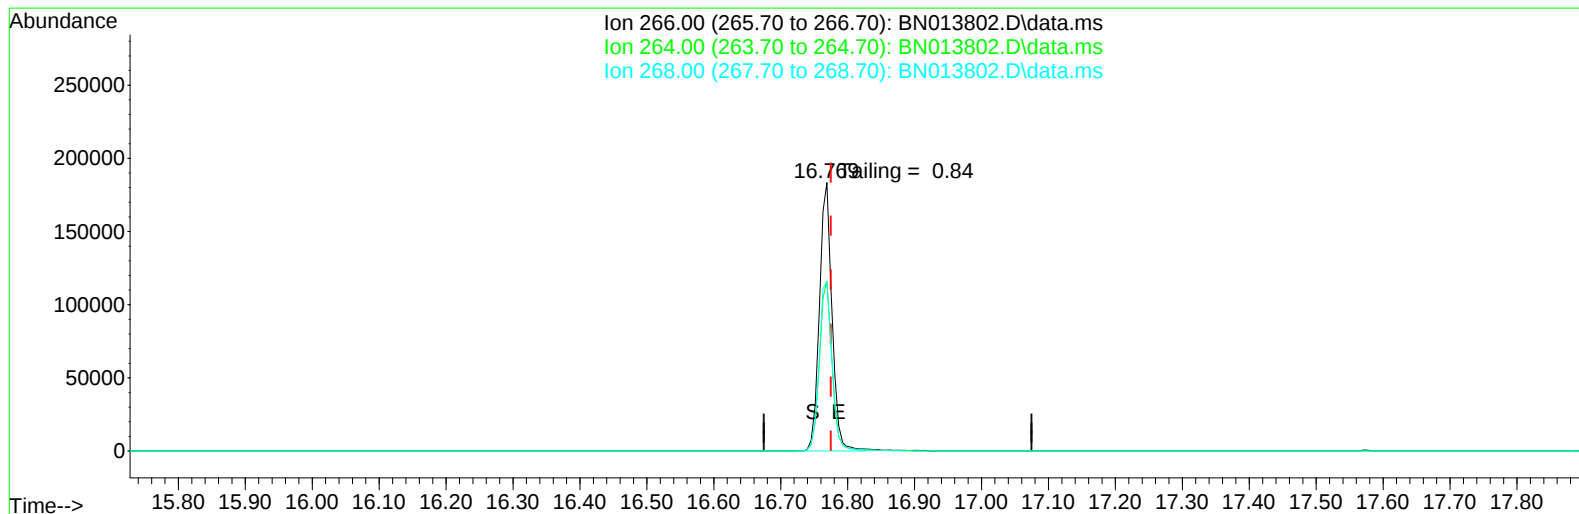

TIC: BN013802.D\data.ms

(24) Pentachlorophenol

16.769min (-0.006) 0.00 ng

response 241790

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	64.50	63.02
268.00	68.30	64.77
0.00	0.00	0.00