
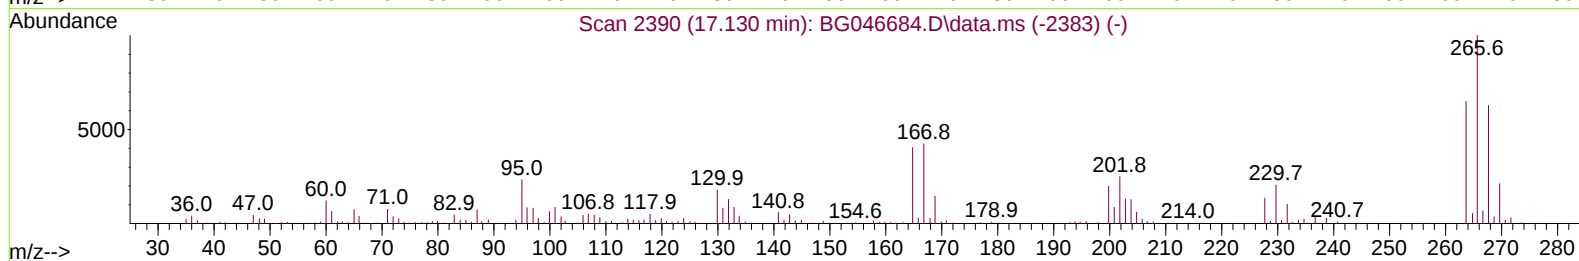
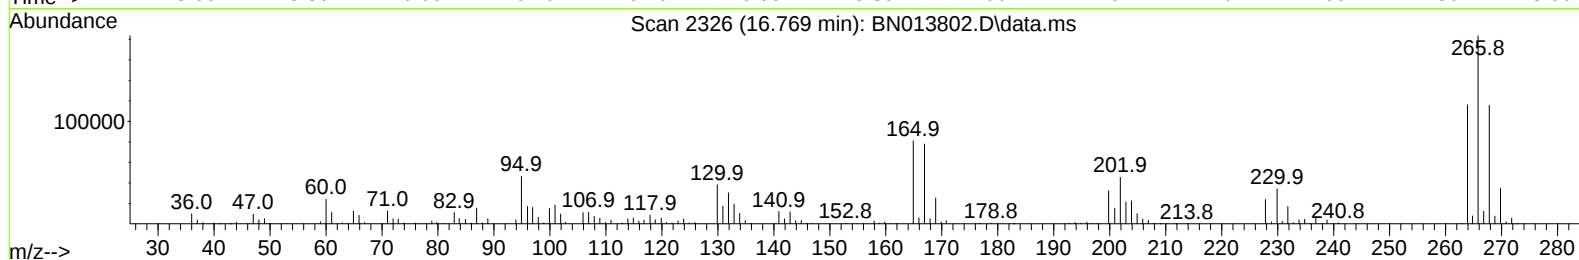


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030221\
Data File : BN013802.D
Acq On : 02 Mar 2021 09:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 03 00:51:31 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 26 07:31:37 2021
Response via : Initial Calibration

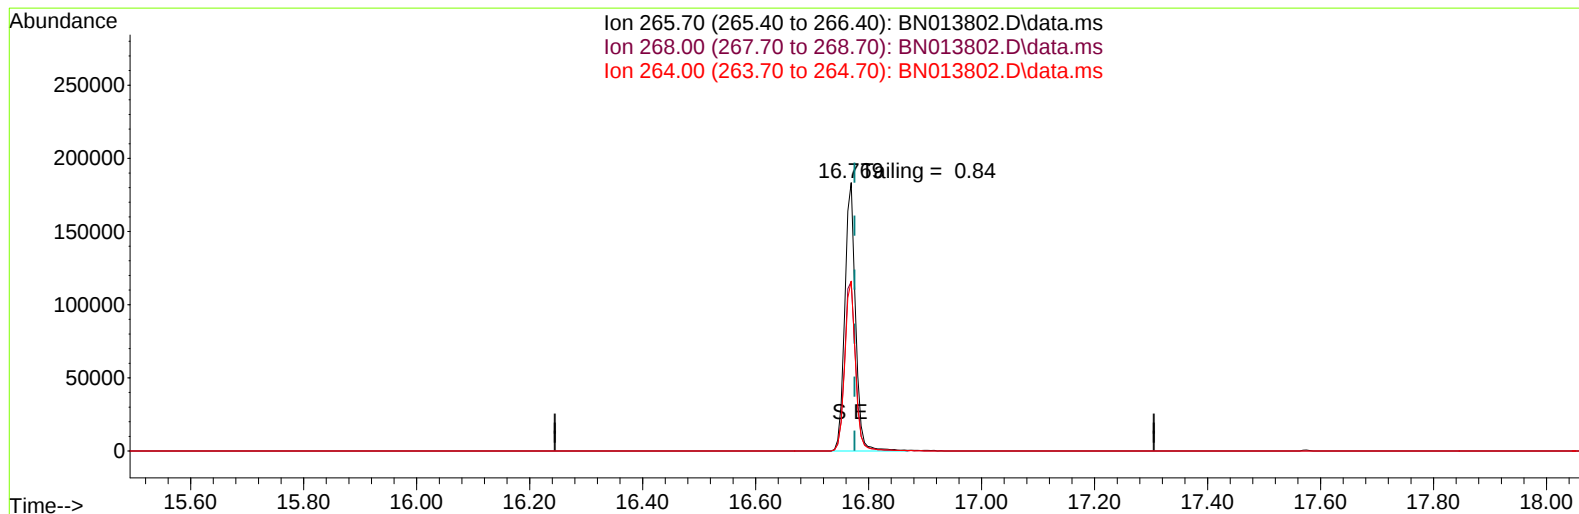

TIC: BN013802.D\data.ms

(70) Pentachlorophenol (C)




16.769min (-0.006) 23976.74 ng

response 241790

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.16
264.00	61.60	63.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030221\
 Data File : BN013802.D
 Acq On : 02 Mar 2021 09:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 03 00:51:31 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 26 07:31:37 2021
 Response via : Initial Calibration

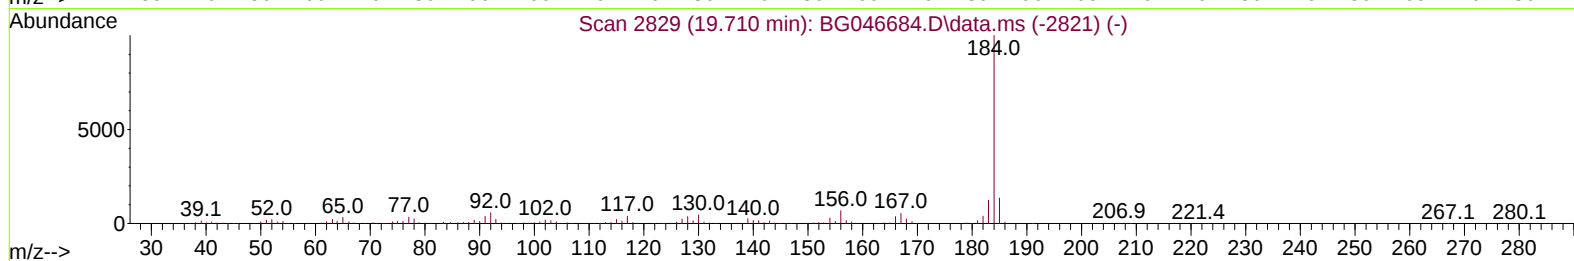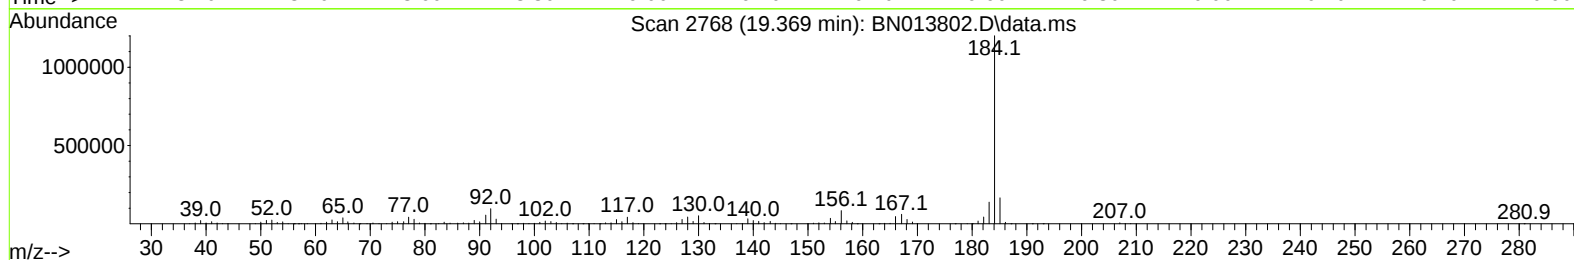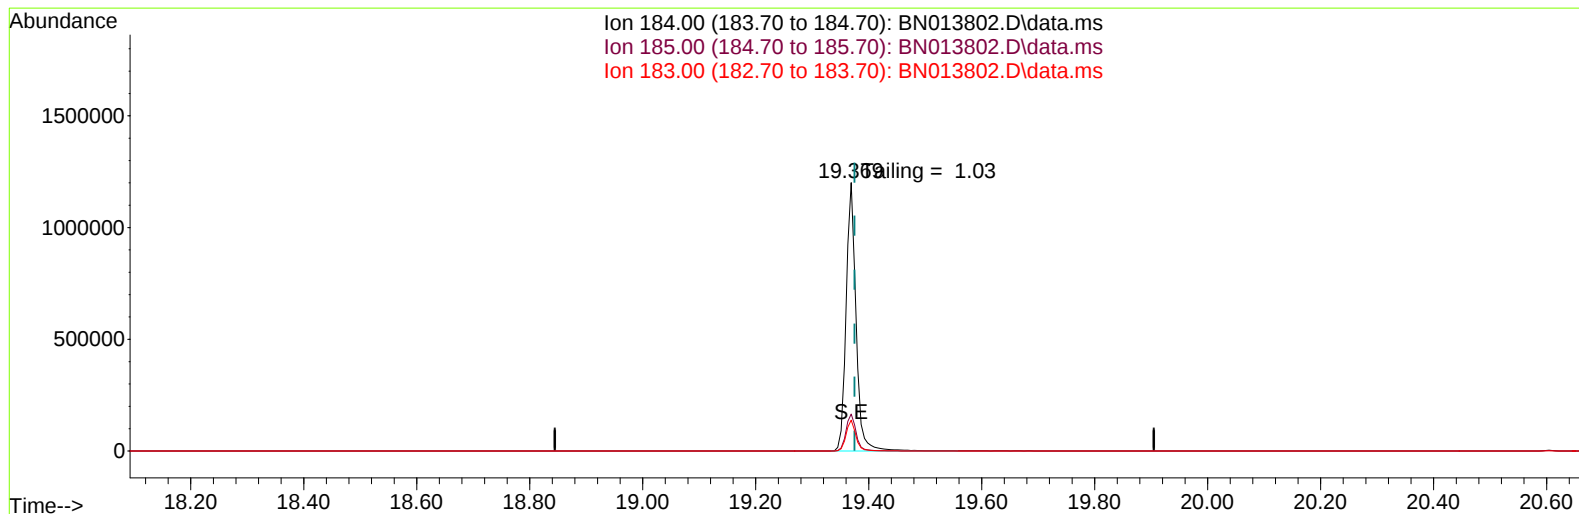

TIC: BN013802.D\data.ms

(77) Benzidine

19.369min (-0.006) 0.00 ng

response 1465554

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.81
183.00	13.20	11.53
0.00	0.00	0.00