
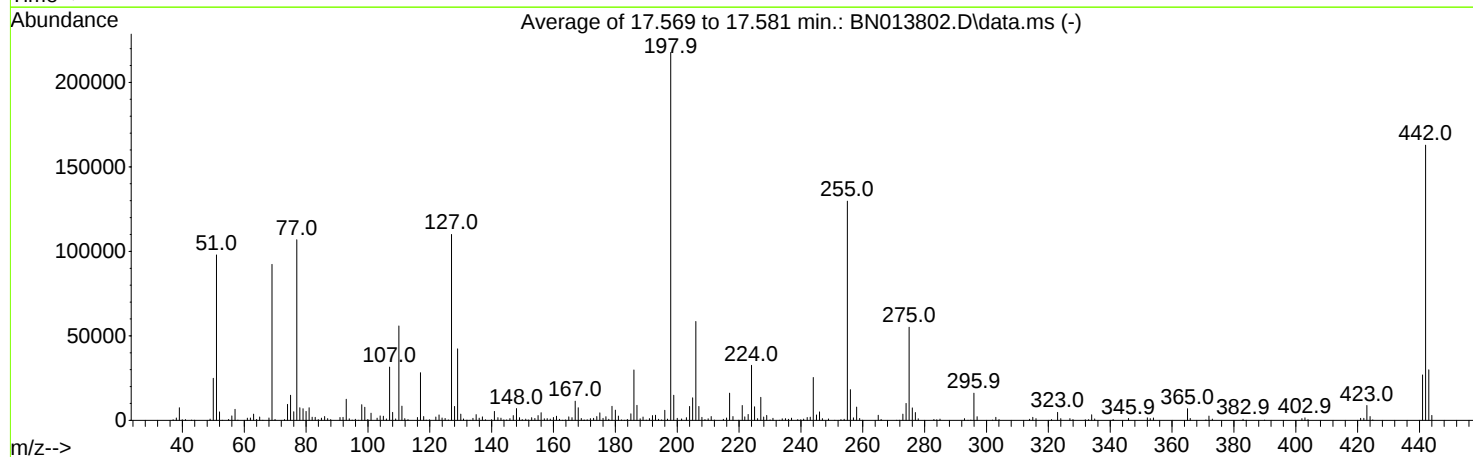


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030221\
 Data File : BN013802.D
 Acq On : 02 Mar 2021 09:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN022421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Feb 25 11:31:11 2021

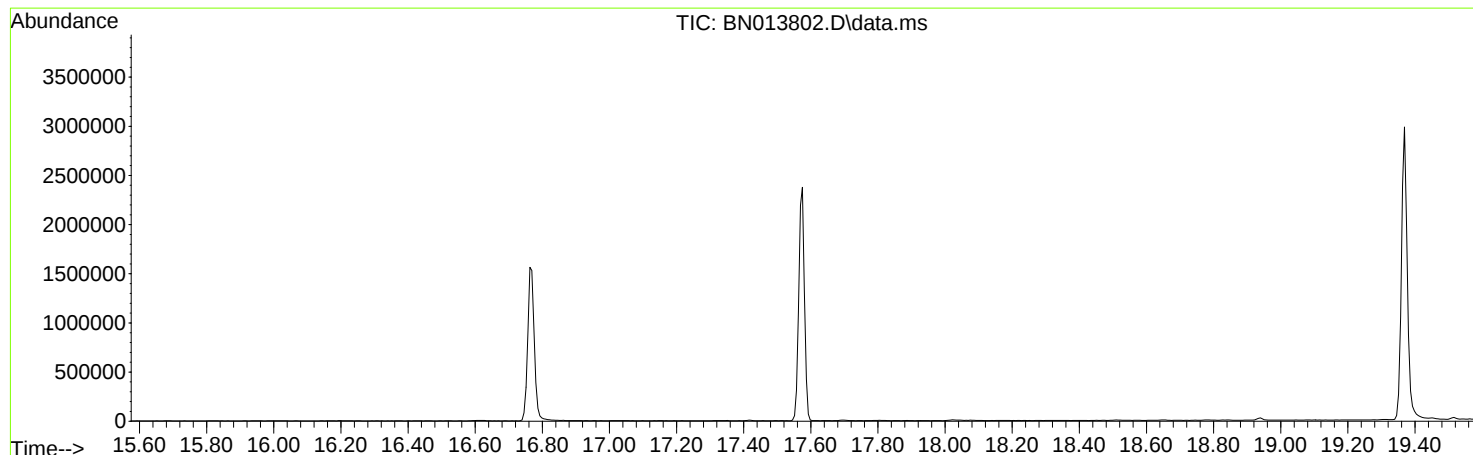

AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.0	97907	PASS
68	69	0.00	2	1.6	1471	PASS
69	198	0.00	100	42.4	92283	PASS
70	69	0.00	2	0.6	566	PASS
127	198	10	80	50.6	110075	PASS
197	198	0.00	2	0.3	758	PASS
198	198	100	100	100.0	217685	PASS
199	198	5	9	6.8	14867	PASS
275	198	10	60	25.3	55069	PASS
365	198	1	100	3.2	6940	PASS
441	198	0.01	100	12.4	26899	PASS
442	442	50	100	100.0	162901	PASS
443	442	15	24	18.4	29957	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/2/2021	BNA_N	<u>BN013802.D</u>
Compound Name	Response	Retention Time
DDT	822138	20.6
DDD	5993	20.16
DDE	1431	19.65
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7424	829562	0.89

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030221\
Data File : BN013802.D
Acq On : 02 Mar 2021 09:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 03 00:51:31 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 26 07:31:37 2021
Response via : Initial Calibration

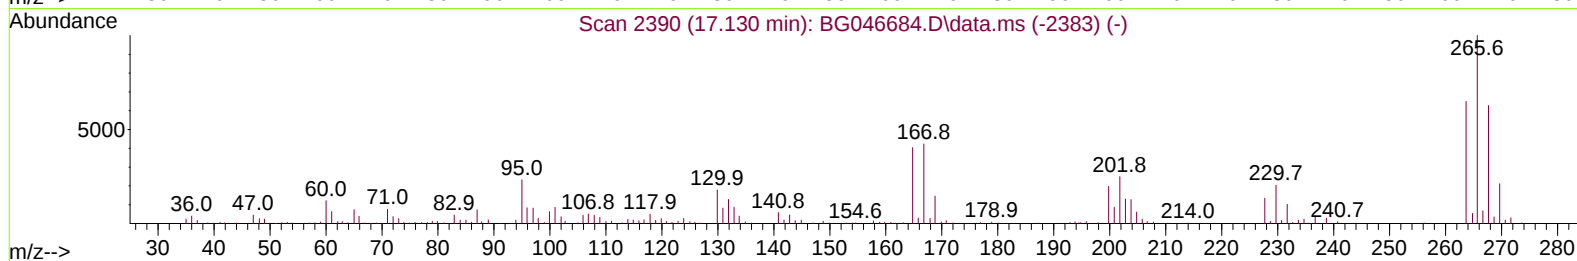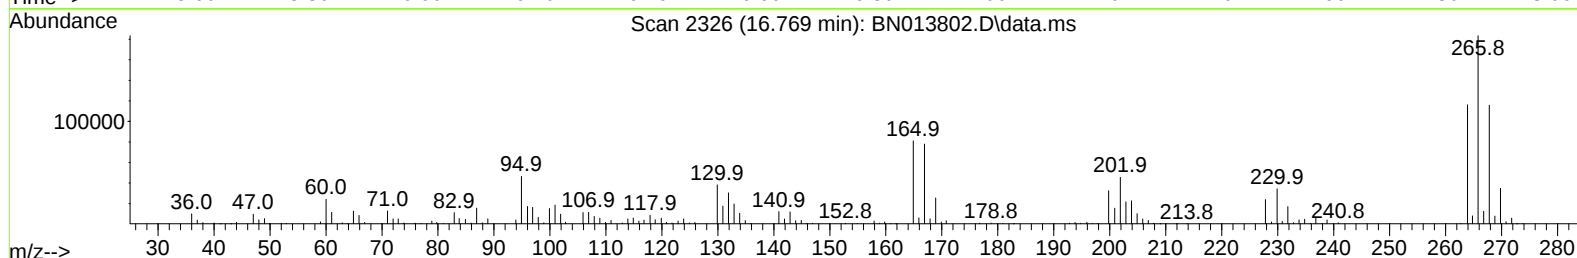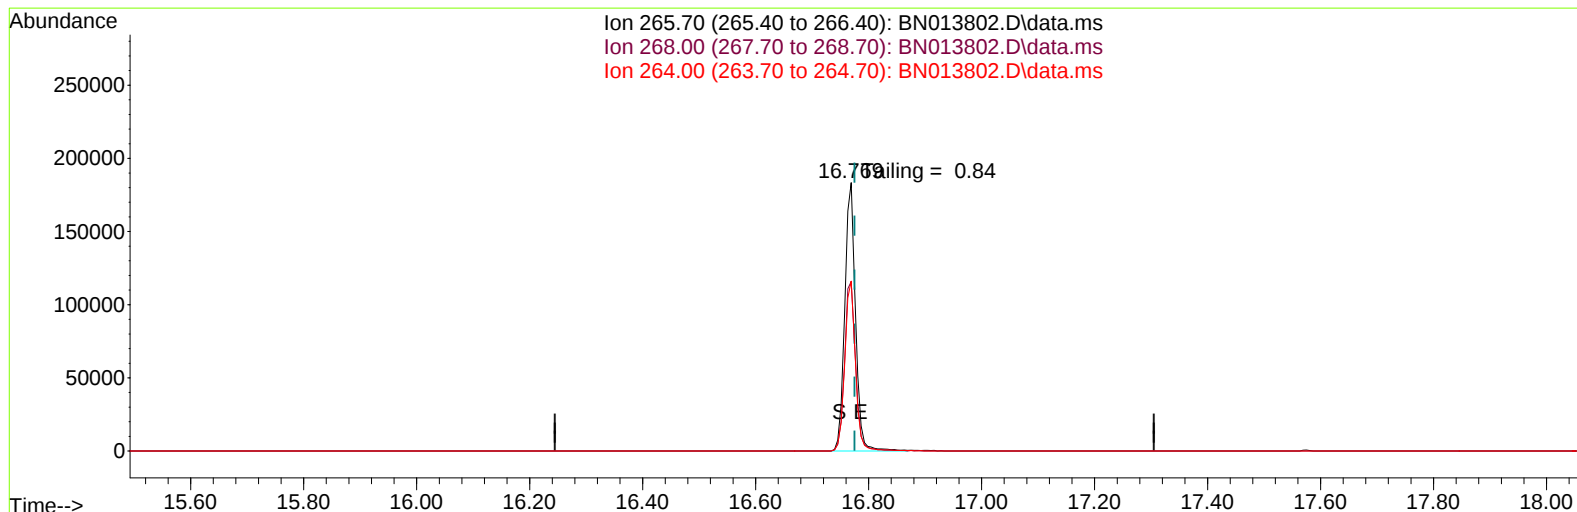

TIC: BN013802.D\data.ms

(70) Pentachlorophenol (C)

16.769min (-0.006) 23976.74 ng




response 241790

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.16
264.00	61.60	63.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030221\
Data File : BN013802.D
Acq On : 02 Mar 2021 09:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 03 00:51:31 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 26 07:31:37 2021
Response via : Initial Calibration

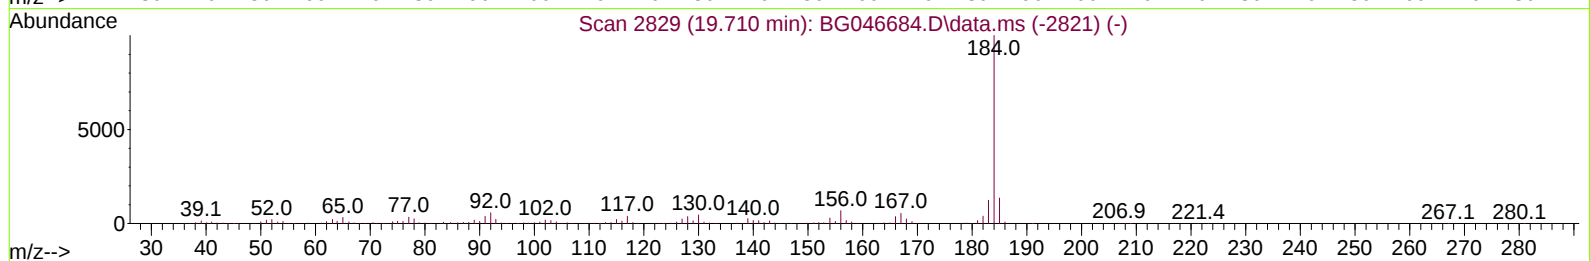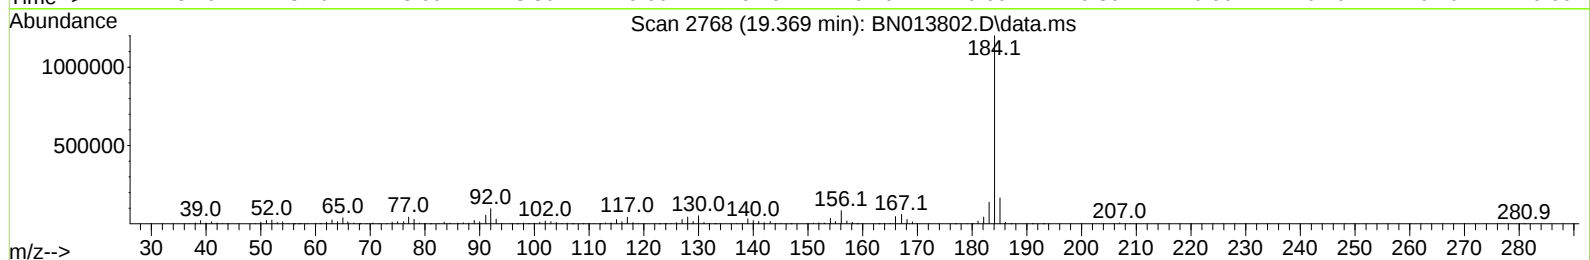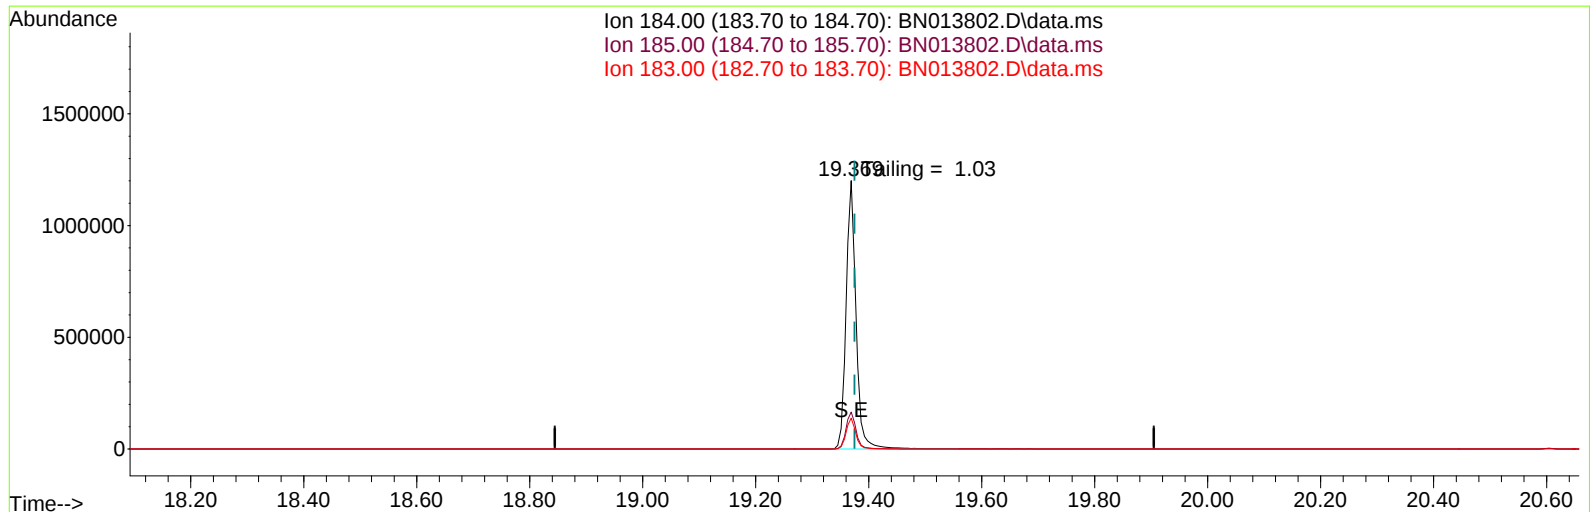

TIC: BN013802.D\data.ms

(77) Benzidine

19.369min (-0.006) 0.00 ng

response 1465554

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.81
183.00	13.20	11.53
0.00	0.00	0.00