

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
 Data File : BN030184.D
 Acq On : 02 Mar 2024 16:55
 Operator : MA/JU
 Sample : PB159333BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK333

Quant Time: Mar 03 22:48:03 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 02 16:09:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.834	152	1389	0.400	ng/ul	0.00
4) Naphthalene-d8	10.628	136	3596	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.479	164	1768	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.234	188	3535	0.400	ng/ul	#-0.01
17) Chrysene-d12	21.459	240	2550	0.400	ng/ul	0.00
23) Perylene-d12	23.797	264	4531	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.302	96	10893	5.665	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.234	152	1476	0.317	ng/ul	0.00
18) Fluoranthene-d10	19.272	212	2811	0.338	ng/ul	-0.01
Target Compounds						
					Qvalue	
12) Fluorene	15.478	166	562	0.076	ng/ul#	19
20) Pyrene	19.639	202	516	0.042	ng/ul#	1
26) Benzo(a)pyrene	23.645	252	1244	0.070	ng/ul#	50


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
Data File : BN030184.D
Acq On : 02 Mar 2024 16:55
Operator : MA/JU
Sample : PB159333BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK333

Quant Time: Mar 03 22:48:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 02 16:09:30 2024
Response via : Initial Calibration




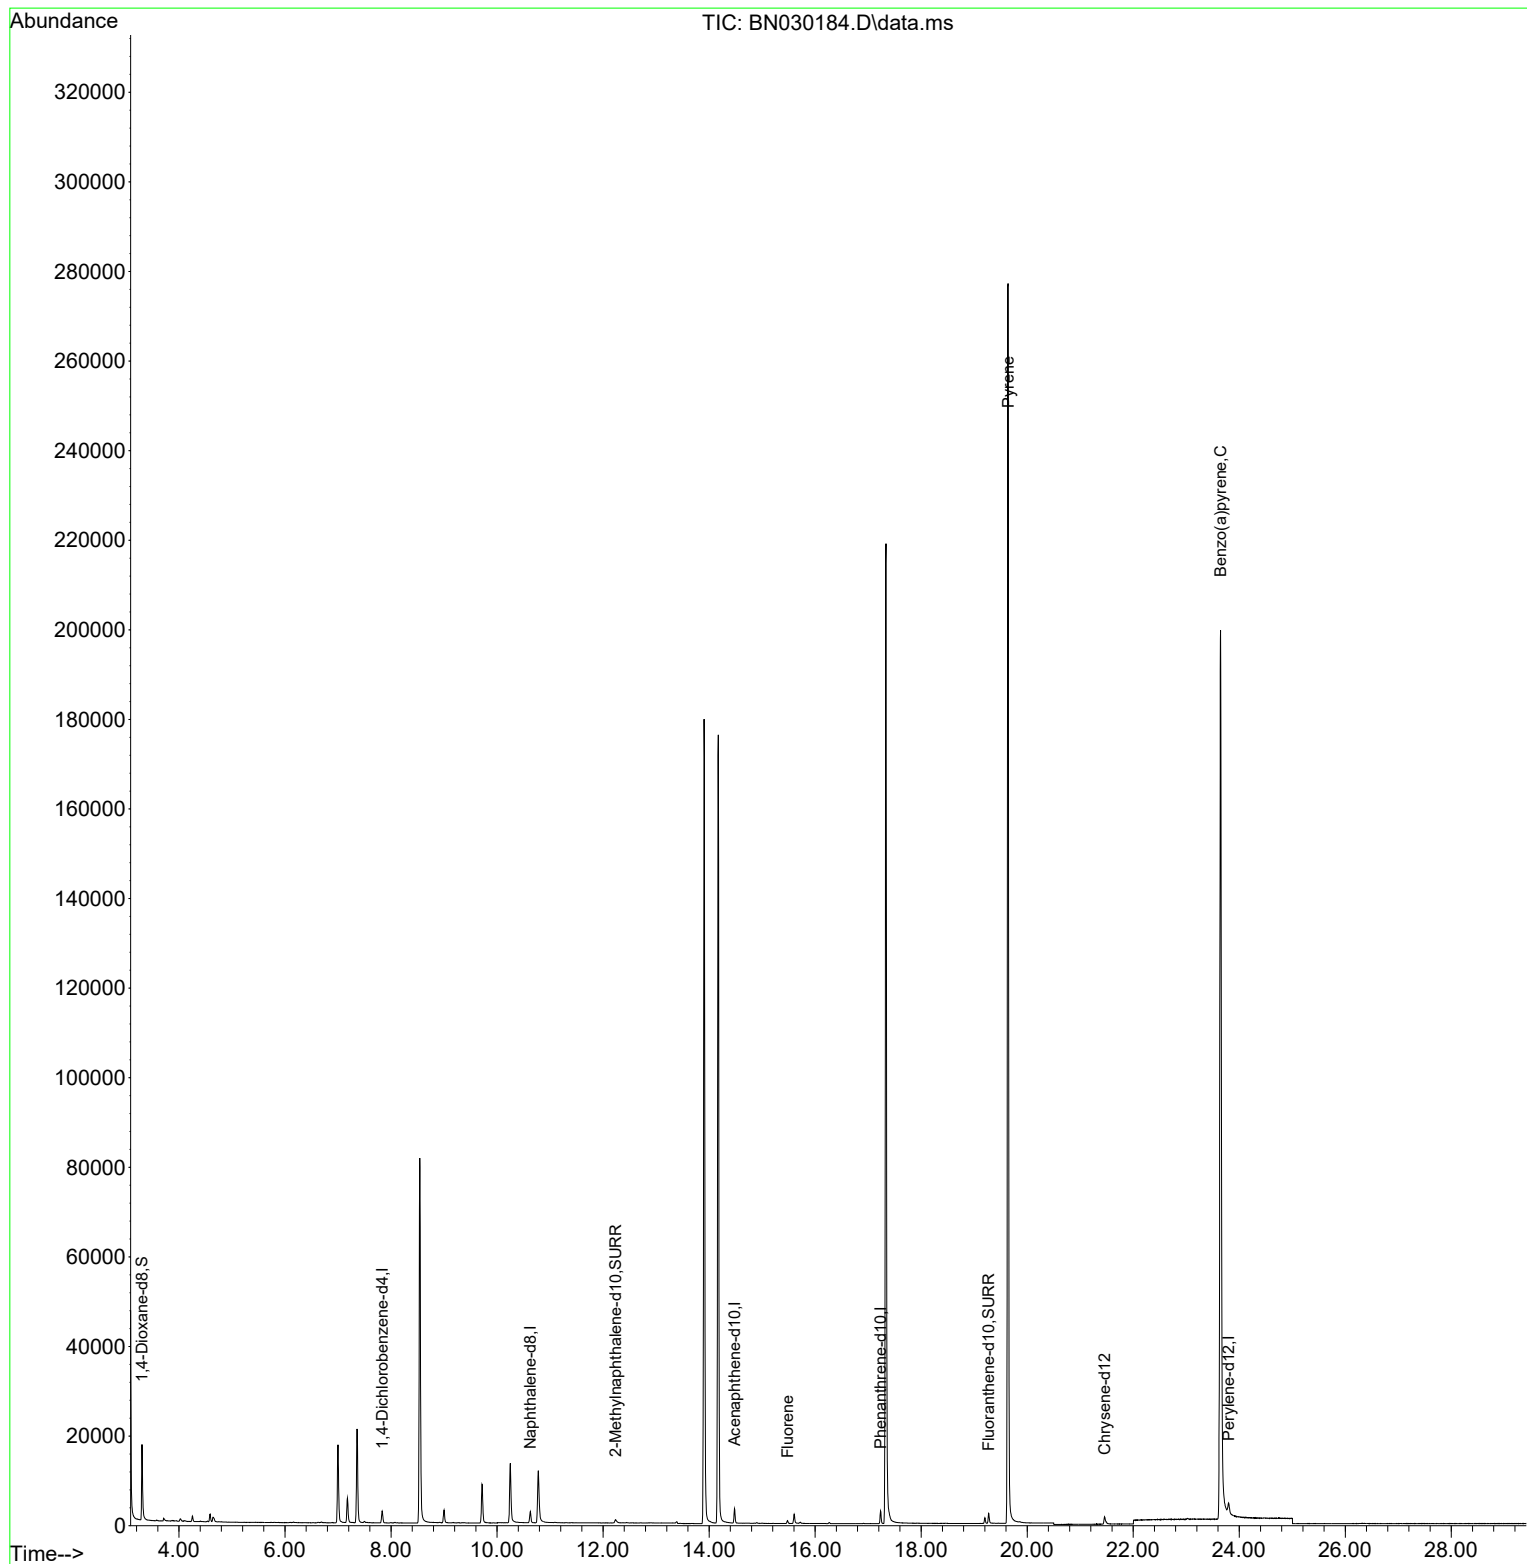


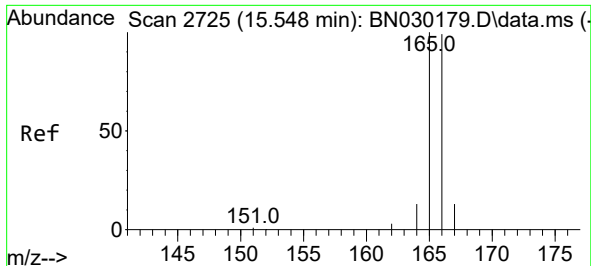

#12
Fluorene
Concen: 0.076 ng/ul
RT: 15.478 min Scan# 21
Delta R.T. -0.070 min
Lab File: BN030184.D
Acq: 02 Mar 2024 16:55




Instrument :
BNA_N
ClientSampleId :
SBLK333


Tgt Ion:166 Resp: 562
Ion Ratio Lower Upper
166 100
165 16.5 81.8 122.6#
167 39.5 13.0 19.4#

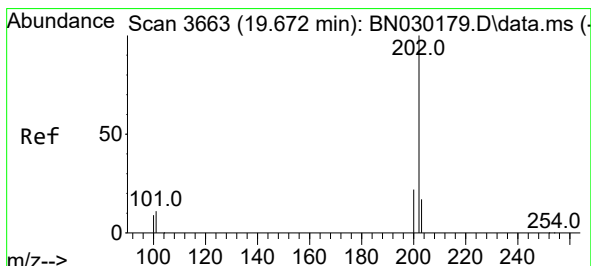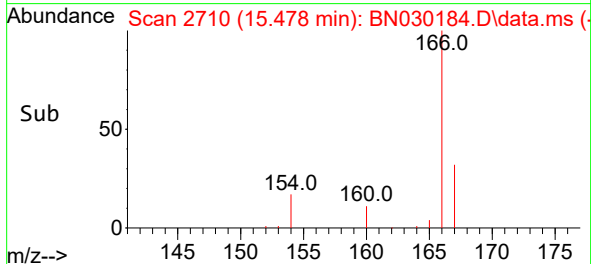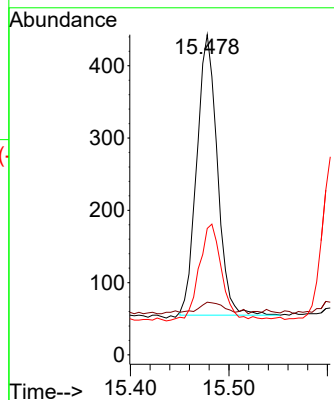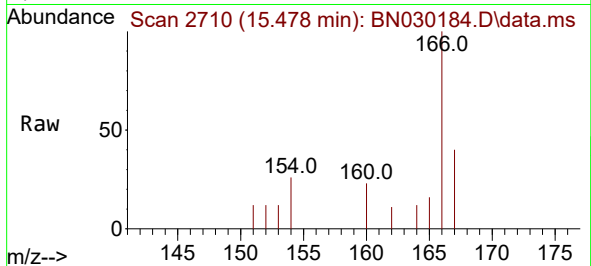

#20
Pyrene
Concen: 0.042 ng/ul
RT: 19.639 min Scan# 3656
Delta R.T. -0.033 min
Lab File: BN030184.D
Acq: 02 Mar 2024 16:55


Tgt Ion:202 Resp: 516
Ion Ratio Lower Upper
202 100
101 220.3 10.6 15.8#
100 1623.0 8.8 13.2#

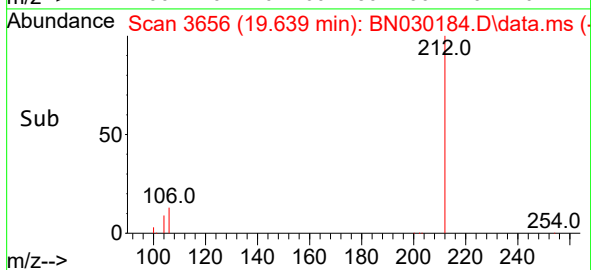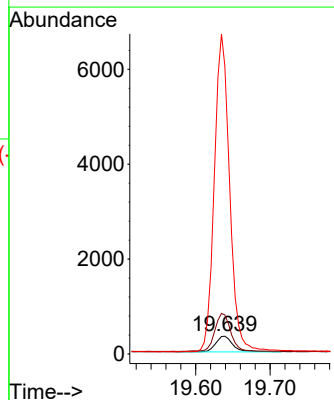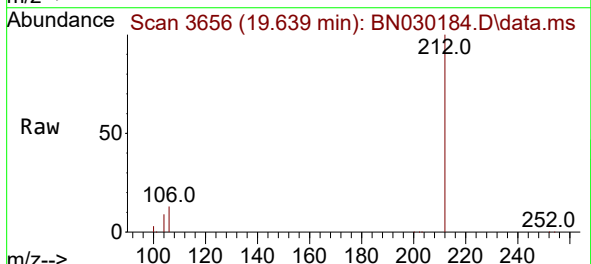

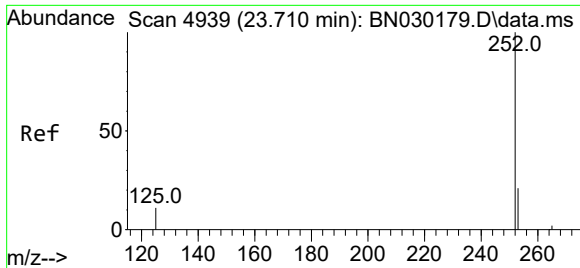

#26
Benzo(a)pyrene
Concen: 0.070 ng/ul
RT: 23.645 min Scan# 4917
Delta R.T. -0.065 min
Lab File: BN030184.D
Acq: 02 Mar 2024 16:55

Instrument :
BNA_N
ClientSampleId :
SBLK333

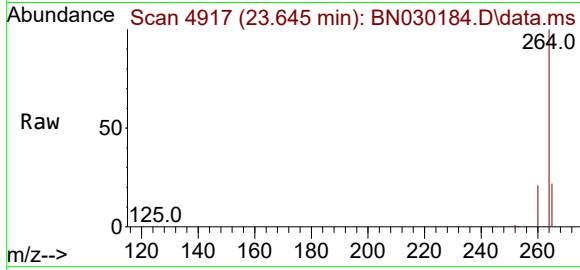

Tgt Ion:252 Resp: 1244
Ion Ratio Lower Upper
252 100
253 71.5 33.0 49.4#
125 46.2 16.9 25.3#

