

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
 Data File : BN030187.D
 Acq On : 02 Mar 2024 18:43
 Operator : MA/JU
 Sample : P1501-17
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E10A4

Quant Time: Mar 03 22:48:32 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 02 16:09:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.834	152	1170	0.400	ng/ul	0.00
4) Naphthalene-d8	10.628	136	3124	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.479	164	1538	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.235	188	3027	0.400	ng/ul	#-0.01
17) Chrysene-d12	21.456	240	2270	0.400	ng/ul	0.00
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.81
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.306	96	8059	4.976	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.234	152	1506	0.373	ng/ul	0.00
18) Fluoranthene-d10	19.273	212	3481	0.471	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.344	88	59	0.034	ng/ul#	72
16) Anthracene	17.332	178	182	0.020	ng/ul#	1
20) Pyrene	19.635	202	618	0.056	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
Data File : BN030187.D
Acq On : 02 Mar 2024 18:43
Operator : MA/JU
Sample : P1501-17
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E10A4

Quant Time: Mar 03 22:48:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 02 16:09:30 2024
Response via : Initial Calibration




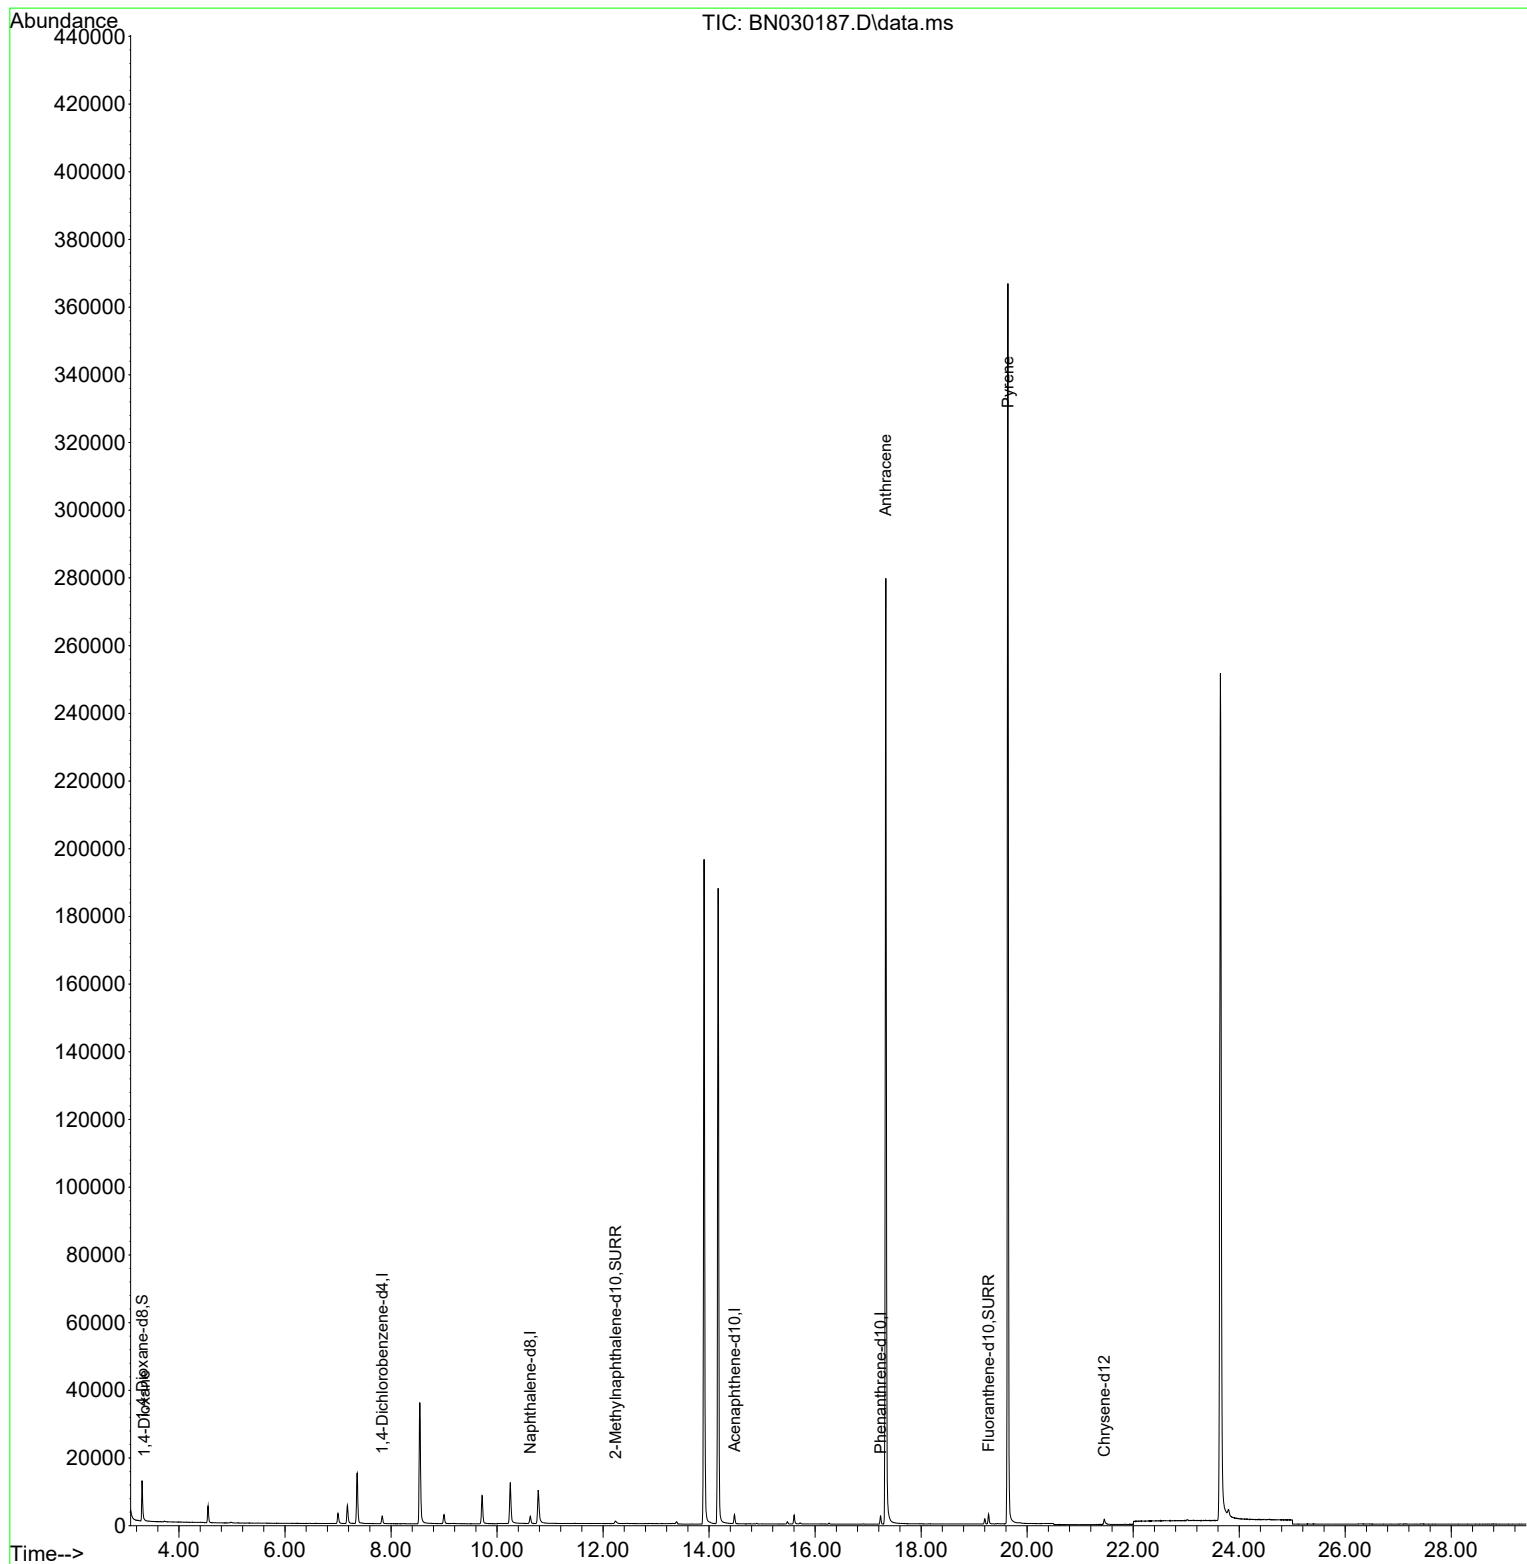


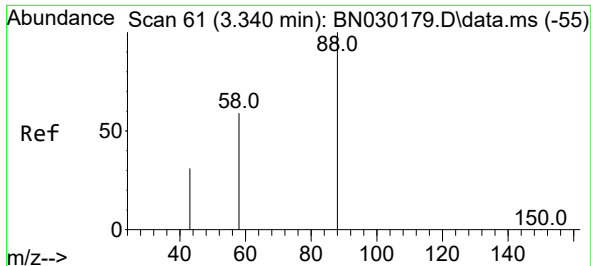

#2
 1,4-Dioxane
 Concen: 0.034 ng/ul
 RT: 3.344 min Scan# 61
 Delta R.T. 0.004 min
 Lab File: BN030187.D
 Acq: 02 Mar 2024 18:43




Instrument :
 BNA_N
 ClientSampleId :
 E10A4


Tgt Ion: 88 Resp: 59
 Ion Ratio Lower Upper
 88 100
 43 37.5 25.7 38.5
 58 15.9 33.8 50.8#

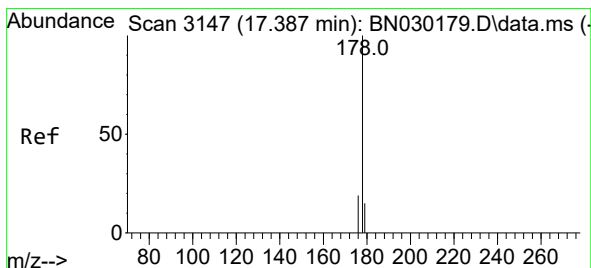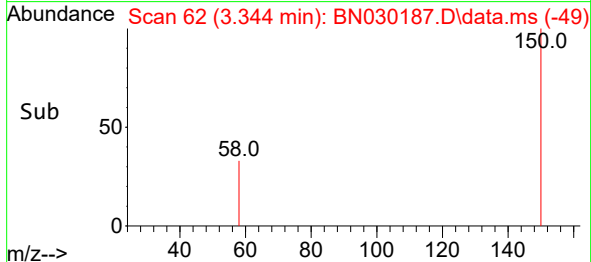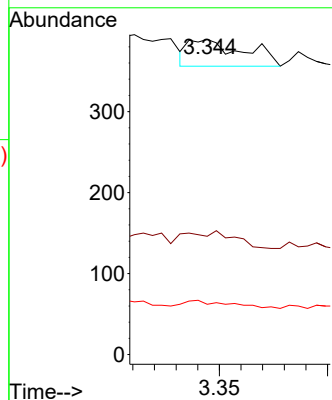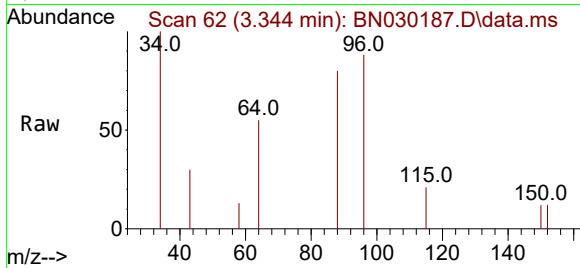

#16
 Anthracene
 Concen: 0.020 ng/ul
 RT: 17.332 min Scan# 3134
 Delta R.T. -0.055 min
 Lab File: BN030187.D
 Acq: 02 Mar 2024 18:43


Tgt Ion: 178 Resp: 182
 Ion Ratio Lower Upper
 178 100
 179 204.6 14.8 22.2#
 176 39.5 17.8 26.6#

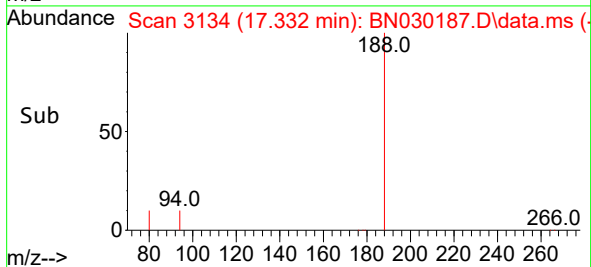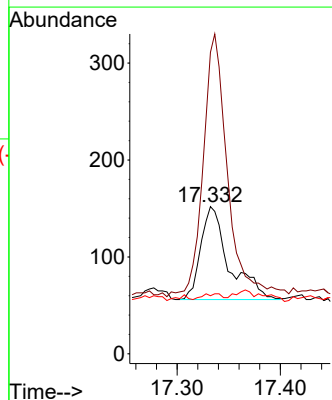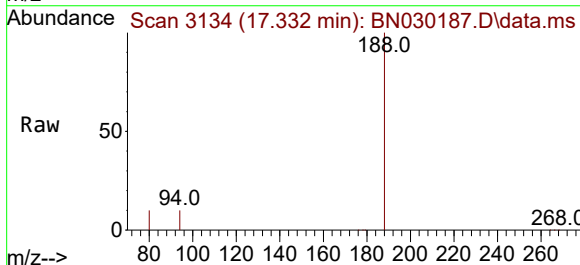

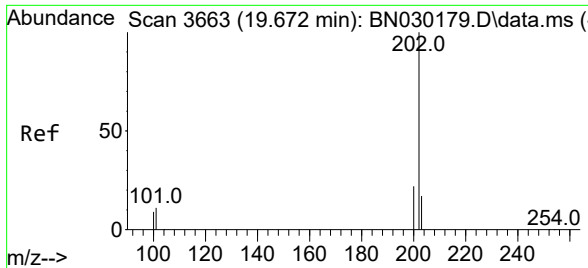

#20
 Pyrene
 Concen: 0.056 ng/ul
 RT: 19.635 min Scan# 30
 Delta R.T. -0.037 min
 Lab File: BN030187.D
 Acq: 02 Mar 2024 18:43

Instrument :
 BNA_N
 ClientSampleId :
 E10A4

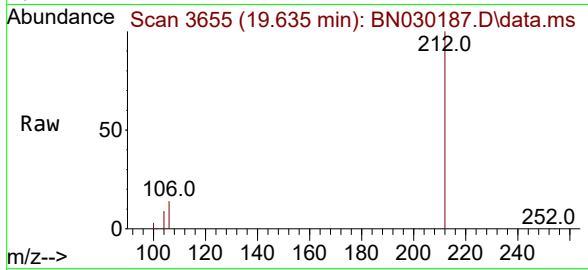

Tgt Ion:202 Resp: 618

Ion	Ratio	Lower	Upper
202	100		
101	239.3	10.6	15.8#
100	1804.4	8.8	13.2#

