

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
 Data File : BN030191.D
 Acq On : 02 Mar 2024 21:43
 Operator : MA/JU
 Sample : PB159249BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK249

Quant Time: Mar 03 22:49:07 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 02 16:09:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.834	152	1566	0.400	ng/ul	0.00
4) Naphthalene-d8	10.628	136	3936	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.479	164	1898	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.235	188	3614	0.400	ng/ul	#-0.01
17) Chrysene-d12	21.459	240	2474	0.400	ng/ul	0.00
23) Perylene-d12	23.797	264	4349	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.303	96	11417	5.266	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.234	152	1472	0.289	ng/ul	0.00
18) Fluoranthene-d10	19.272	212	2688	0.333	ng/ul	0.00
Target Compounds						Qvalue
20) Pyrene	19.635	202	482	0.040	ng/ul#	1
26) Benzo(a)pyrene	23.642	252	1134	0.066	ng/ul#	48


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
Data File : BN030191.D
Acq On : 02 Mar 2024 21:43
Operator : MA/JU
Sample : PB159249BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK249

Quant Time: Mar 03 22:49:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 02 16:09:30 2024
Response via : Initial Calibration




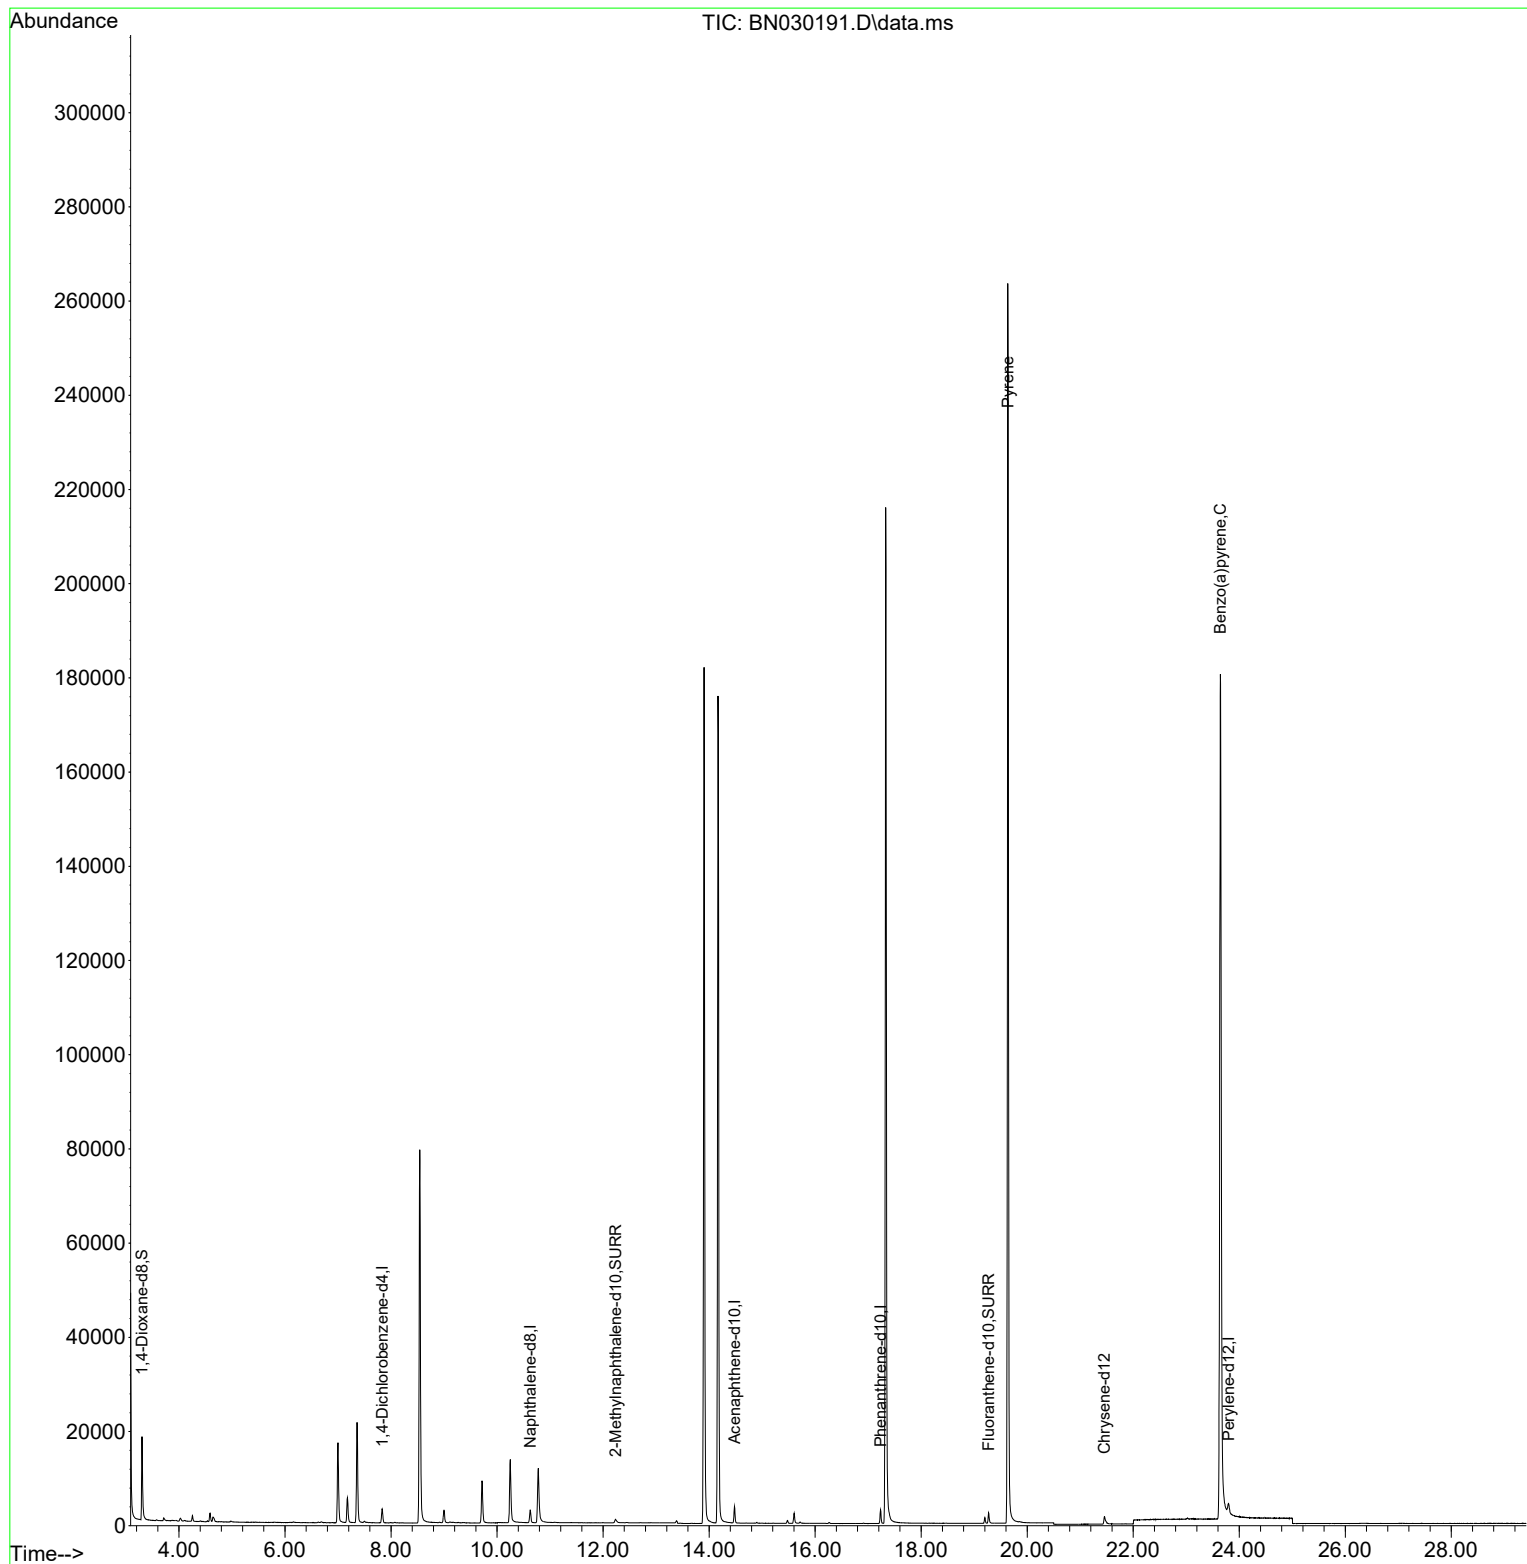


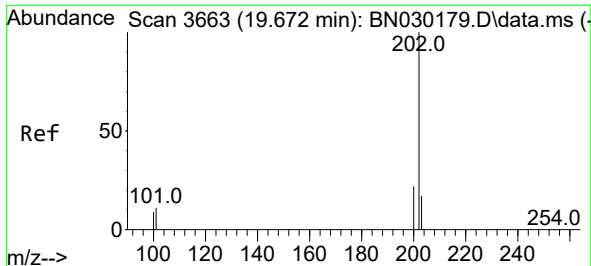

#20
Pyrene
Concen: 0.040 ng/ul
RT: 19.635 min Scan# 301
Delta R.T. -0.038 min
Lab File: BN030191.D
Acq: 02 Mar 2024 21:43

Instrument :
BNA_N
ClientSampleId :
SBLK249

Tgt Ion:202 Resp: 482
Ion Ratio Lower Upper
202 100
101 218.4 10.6 15.8#
100 1661.4 8.8 13.2#

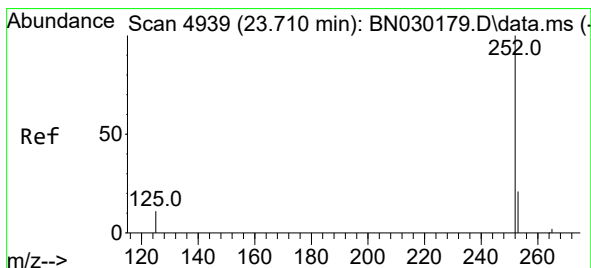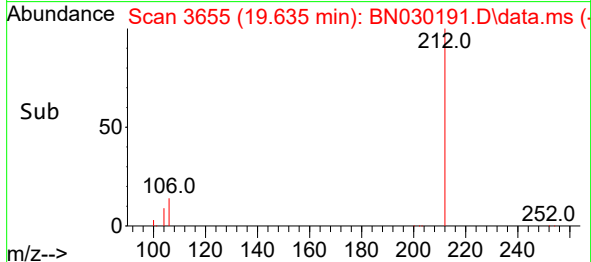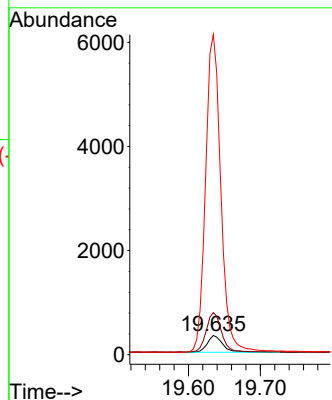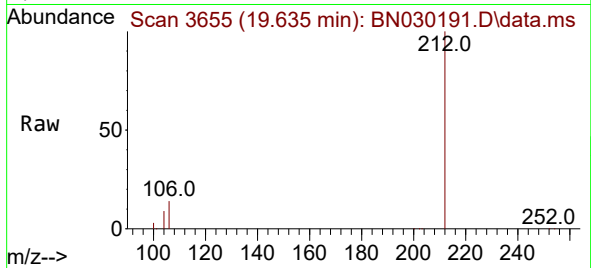

#26
Benzo(a)pyrene
Concen: 0.066 ng/ul
RT: 23.642 min Scan# 4916
Delta R.T. -0.068 min
Lab File: BN030191.D
Acq: 02 Mar 2024 21:43

Tgt Ion:252 Resp: 1134
Ion Ratio Lower Upper
252 100
253 73.6 33.0 49.4#
125 45.4 16.9 25.3#

