

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
 Data File : BN030193.D
 Acq On : 02 Mar 2024 22:56
 Operator : MA/JU
 Sample : P1501-20
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E10B9

Quant Time: Mar 03 22:49:21 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 02 16:09:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.834	152	1082	0.400	ng/ul	0.00
4) Naphthalene-d8	10.623	136	2876	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.479	164	1474	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.235	188	2852	0.400	ng/ul	#-0.01
17) Chrysene-d12	21.456	240	2139	0.400	ng/ul	0.00
23) Perylene-d12	23.794	264	3563	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.302	96	7910	5.281	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.234	152	1744	0.469	ng/ul	0.00
18) Fluoranthene-d10	19.272	212	3716	0.533	ng/ul	0.00
Target Compounds						Qvalue
20) Pyrene	19.635	202	754	0.073	ng/ul#	1
26) Benzo(a)pyrene	23.645	252	1671	0.119	ng/ul#	58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
Data File : BN030193.D
Acq On : 02 Mar 2024 22:56
Operator : MA/JU
Sample : P1501-20
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E10B9

Quant Time: Mar 03 22:49:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 02 16:09:30 2024
Response via : Initial Calibration

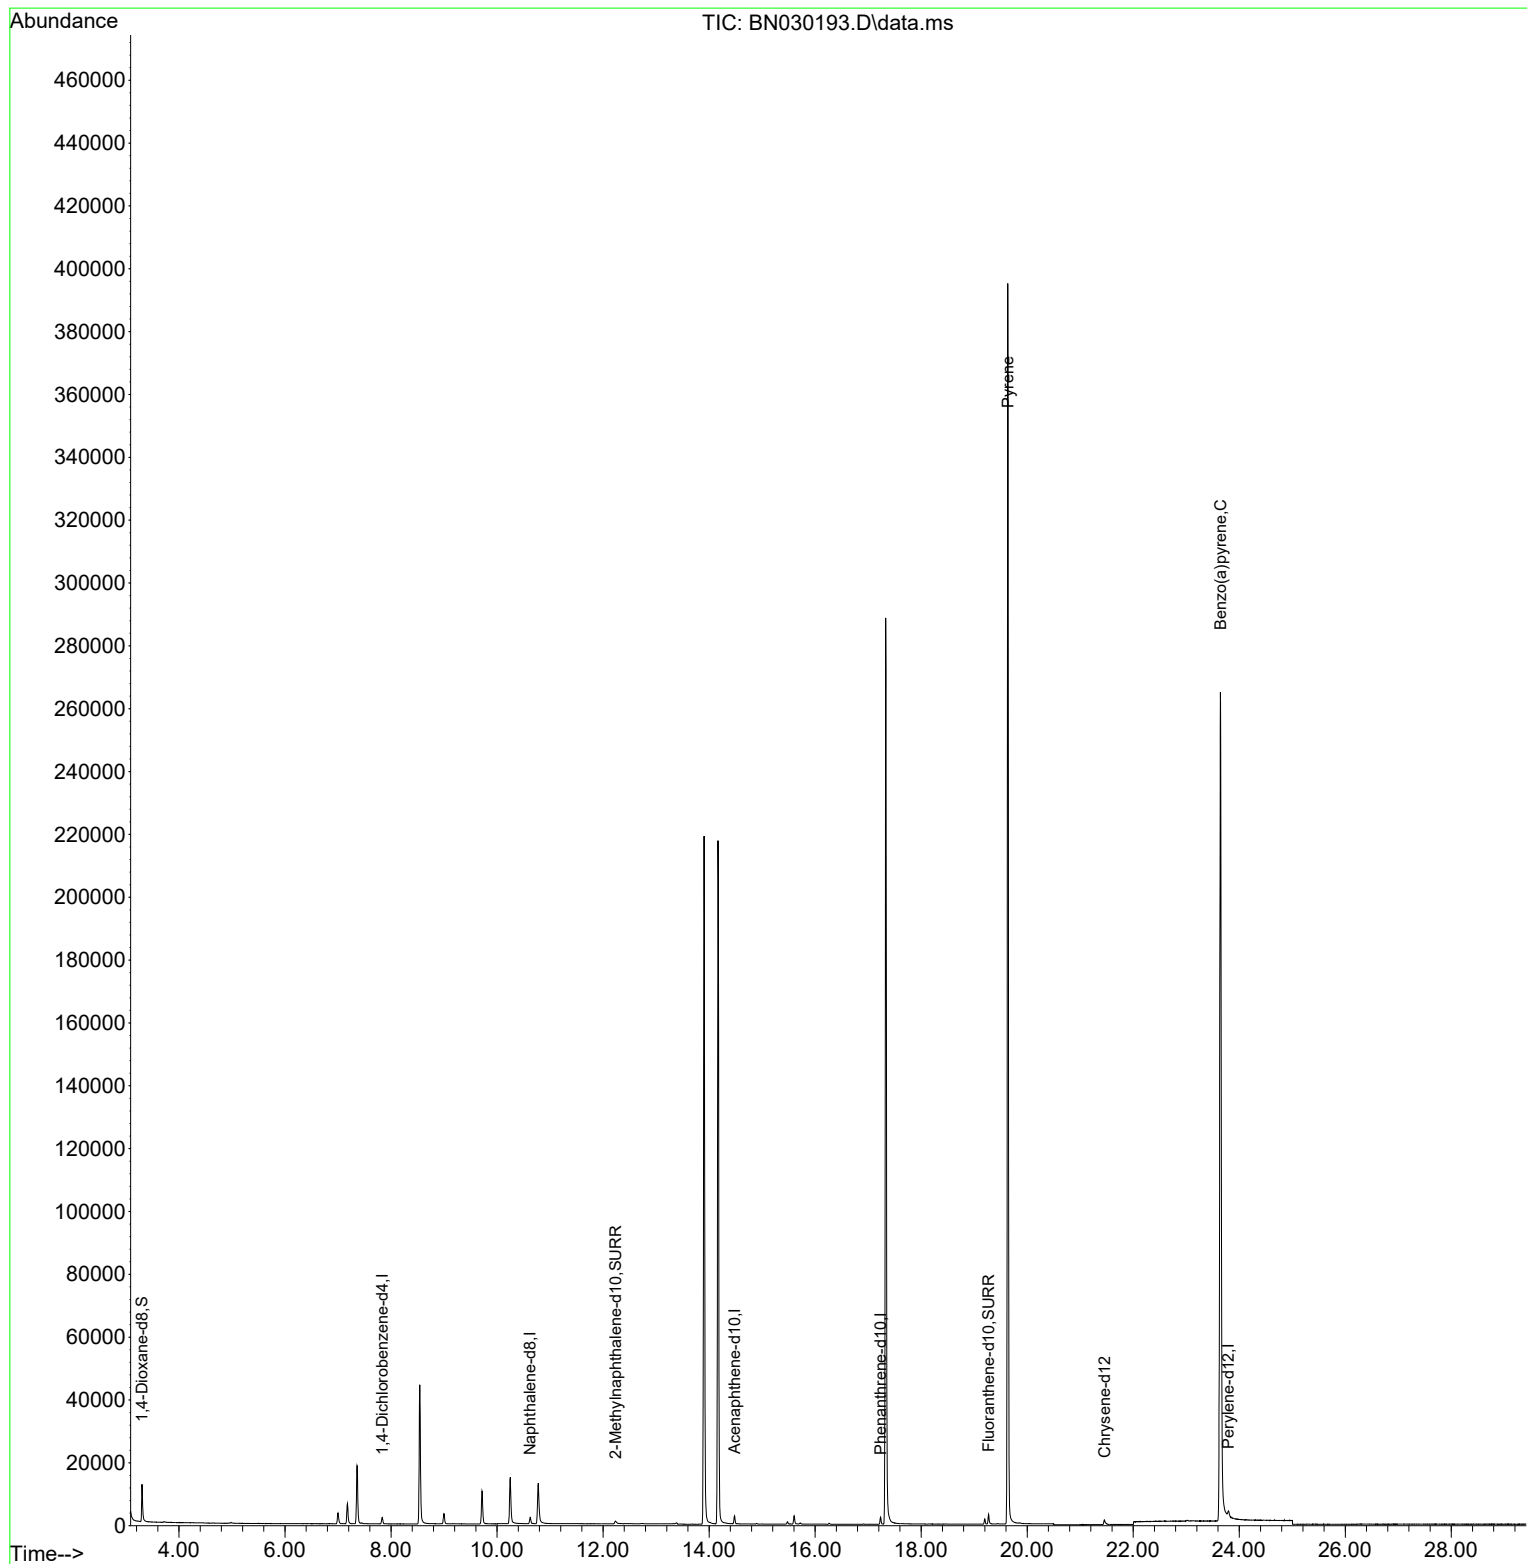

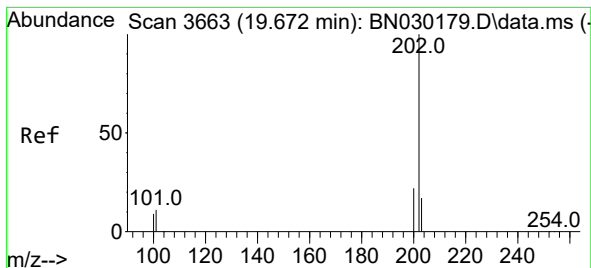

#20

Pyrene

Concen: 0.073 ng/ul

RT: 19.635 min Scan# 30

Delta R.T. -0.038 min

Lab File: BN030193.D

Acq: 02 Mar 2024 22:56

Instrument :

BNA_N

ClientSampleId :

E10B9





Tgt Ion:202 Resp: 754

Ion Ratio Lower Upper

202 100

101 229.3 10.6 15.8#

100 1812.3 8.8 13.2#

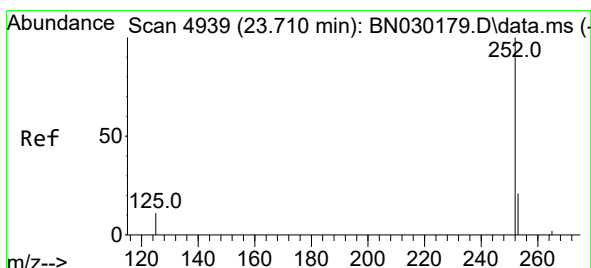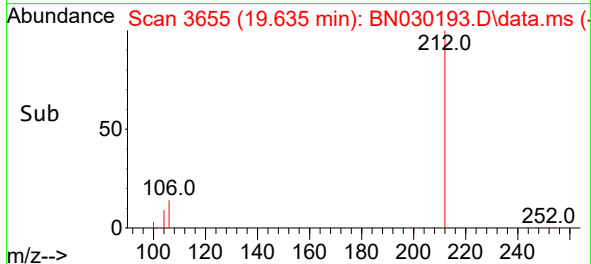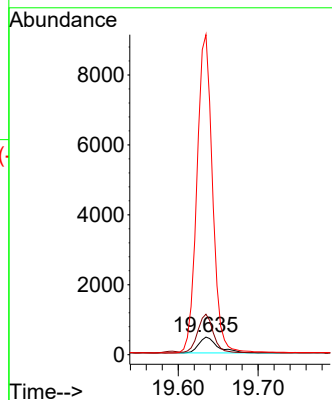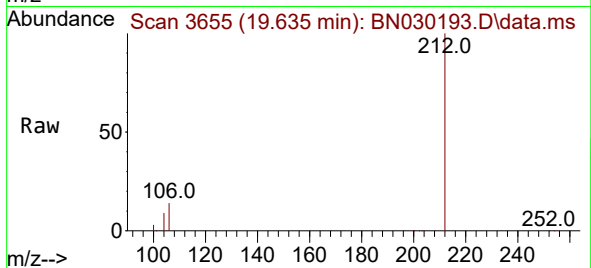

#26

Benzo(a)pyrene

Concen: 0.119 ng/ul

RT: 23.645 min Scan# 4917

Delta R.T. -0.065 min

Lab File: BN030193.D

Acq: 02 Mar 2024 22:56

Tgt Ion:252 Resp: 1671

Ion Ratio Lower Upper

252 100

253 64.5 33.0 49.4#

125 44.5 16.9 25.3#

