

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
 Data File : BN030198.D
 Acq On : 03 Mar 2024 01:56
 Operator : MA/JU
 Sample : P1501-12
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E10B3

Quant Time: Mar 03 22:50:02 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 02 16:09:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.834	152	1375	0.400	ng/ul	0.00
4) Naphthalene-d8	10.628	136	3653	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.479	164	1891	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.235	188	3792	0.400	ng/ul	#-0.01
17) Chrysene-d12	21.453	240	2944	0.400	ng/ul	# 0.00
23) Perylene-d12	23.794	264	4921	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.302	96	7606	3.996	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.234	152	1410	0.299	ng/ul	0.00
18) Fluoranthene-d10	19.272	212	3665	0.382	ng/ul	0.00
Target Compounds						
					Qvalue	
11) Acenaphthene	14.567	153	583	0.075	ng/ul#	33
20) Pyrene	19.635	202	644	0.045	ng/ul#	1
26) Benzo(a)pyrene	23.642	252	1541	0.080	ng/ul#	60


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
Data File : BN030198.D
Acq On : 03 Mar 2024 01:56
Operator : MA/JU
Sample : P1501-12
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E10B3

Quant Time: Mar 03 22:50:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 02 16:09:30 2024
Response via : Initial Calibration




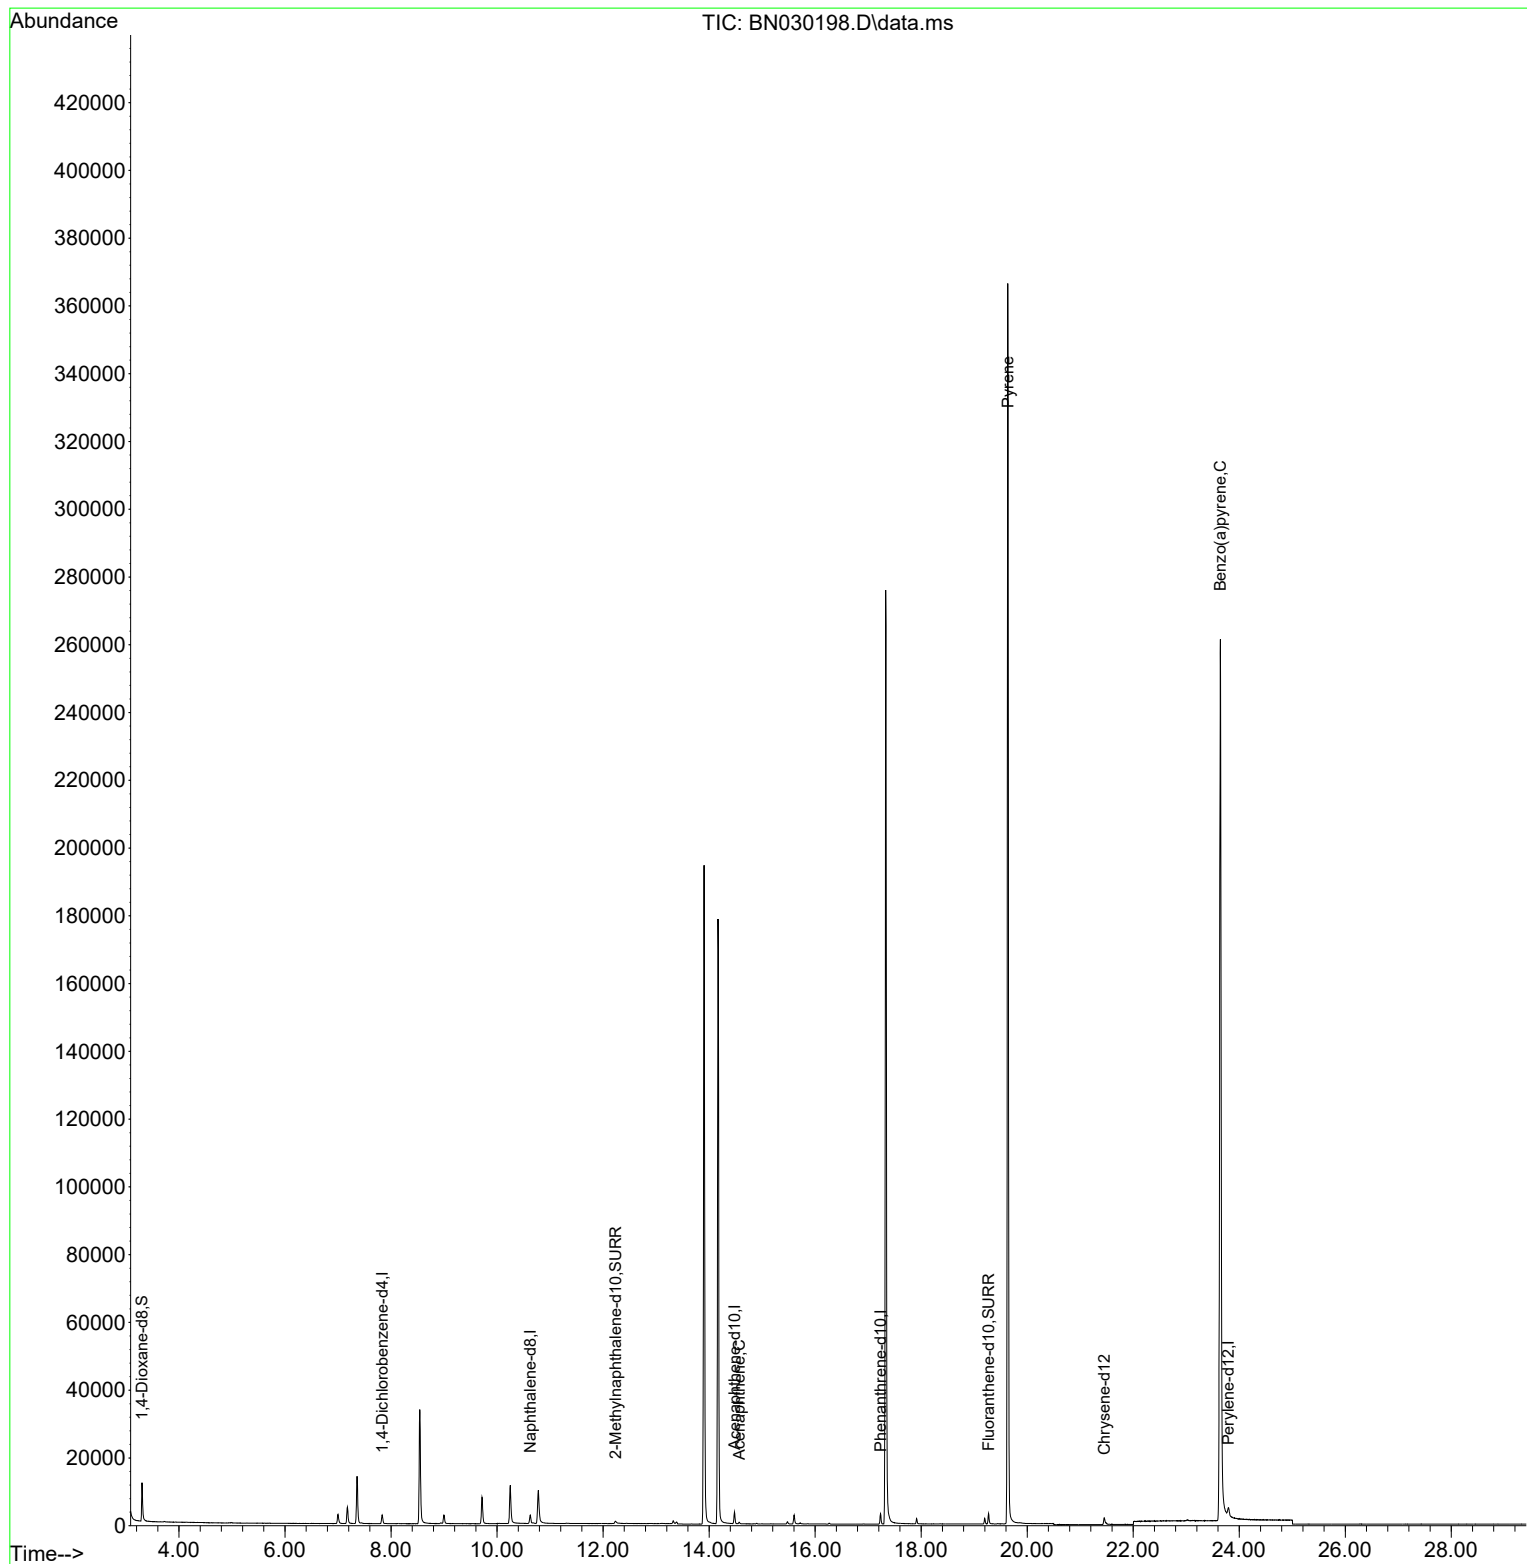


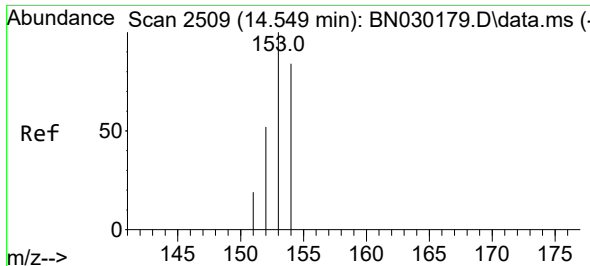

#11
Acenaphthene
Concen: 0.075 ng/ul
RT: 14.567 min Scan# 211
Delta R.T. 0.018 min
Lab File: BN030198.D
Acq: 03 Mar 2024 01:56




Instrument :
BNA_N
ClientSampleId :
E10B3


Tgt Ion:153 Resp: 583
Ion Ratio Lower Upper
153 100
152 11.7 43.2 64.8#
154 18.3 67.5 101.3#

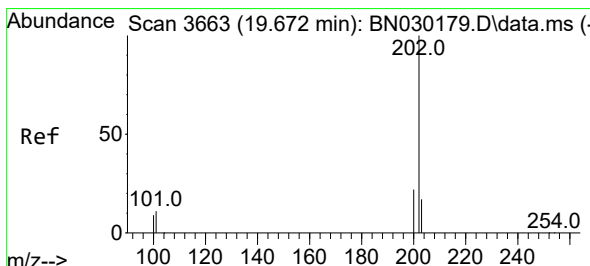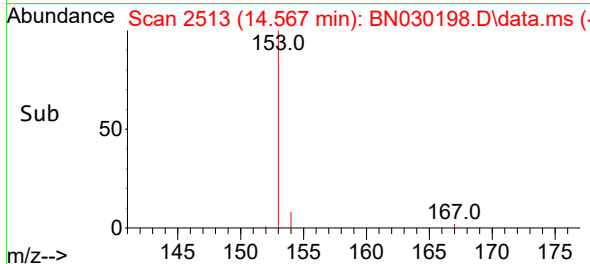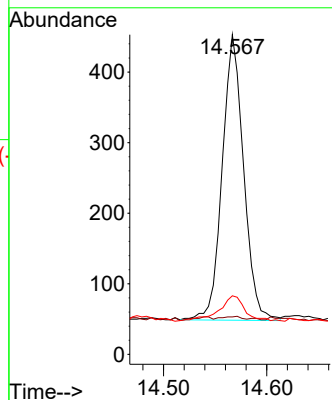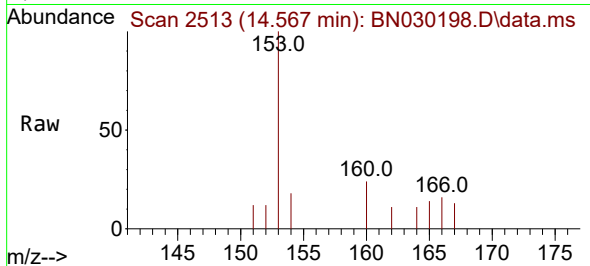

#20
Pyrene
Concen: 0.045 ng/ul
RT: 19.635 min Scan# 3655
Delta R.T. -0.038 min
Lab File: BN030198.D
Acq: 03 Mar 2024 01:56


Tgt Ion:202 Resp: 644
Ion Ratio Lower Upper
202 100
101 218.4 10.6 15.8#
100 1735.4 8.8 13.2#

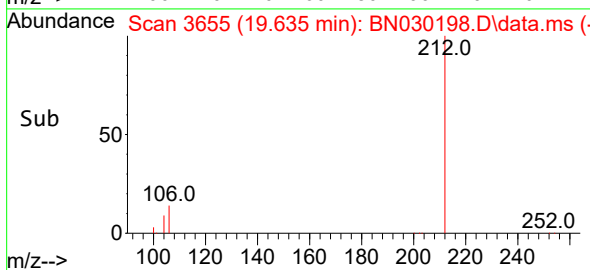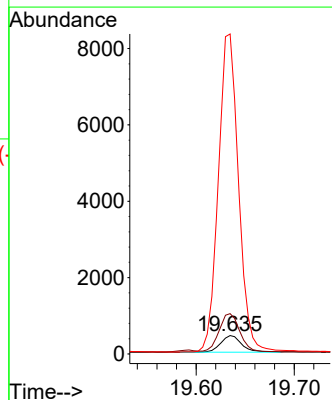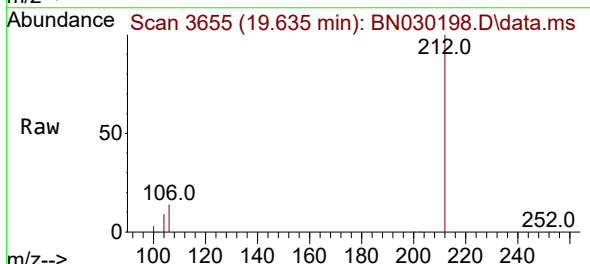

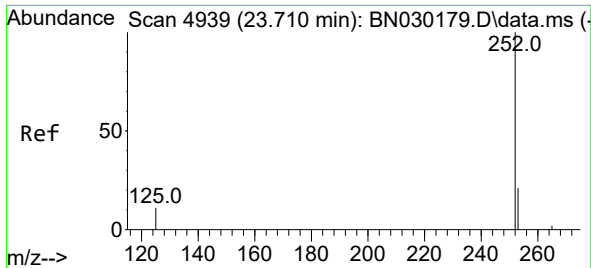

#26
Benzo(a)pyrene
Concen: 0.080 ng/ul
RT: 23.642 min Scan# 4916
Delta R.T. -0.068 min
Lab File: BN030198.D
Acq: 03 Mar 2024 01:56

Instrument :
BNA_N
ClientSampleId :
E10B3

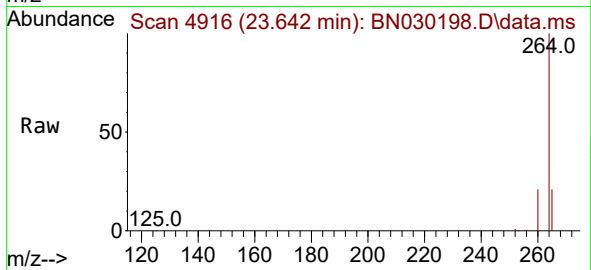

Tgt Ion:252 Resp: 1541
Ion Ratio Lower Upper
252 100
253 64.1 33.0 49.4#
125 43.5 16.9 25.3#

