

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
 Data File : BN030200.D
 Acq On : 03 Mar 2024 03:09
 Operator : MA/JU
 Sample : P1501-15
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E10A2

Quant Time: Mar 03 22:50:16 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 02 16:09:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.834	152	1681	0.400	ng/ul	0.00
4) Naphthalene-d8	10.628	136	4435	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.479	164	2174	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.234	188	4402	0.400	ng/ul	#-0.01
17) Chrysene-d12	21.450	240	3410	0.400	ng/ul	# 0.00
23) Perylene-d12	23.794	264	5638	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.302	96	7222	3.103	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.234	152	1770	0.309	ng/ul	0.00
18) Fluoranthene-d10	19.272	212	4047	0.364	ng/ul	-0.01
Target Compounds						
					Qvalue	
20) Pyrene	19.634	202	727	0.044	ng/ul#	1
26) Benzo(a)pyrene	23.642	252	1686	0.076	ng/ul#	61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
Data File : BN030200.D
Acq On : 03 Mar 2024 03:09
Operator : MA/JU
Sample : P1501-15
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E10A2

Quant Time: Mar 03 22:50:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 02 16:09:30 2024
Response via : Initial Calibration

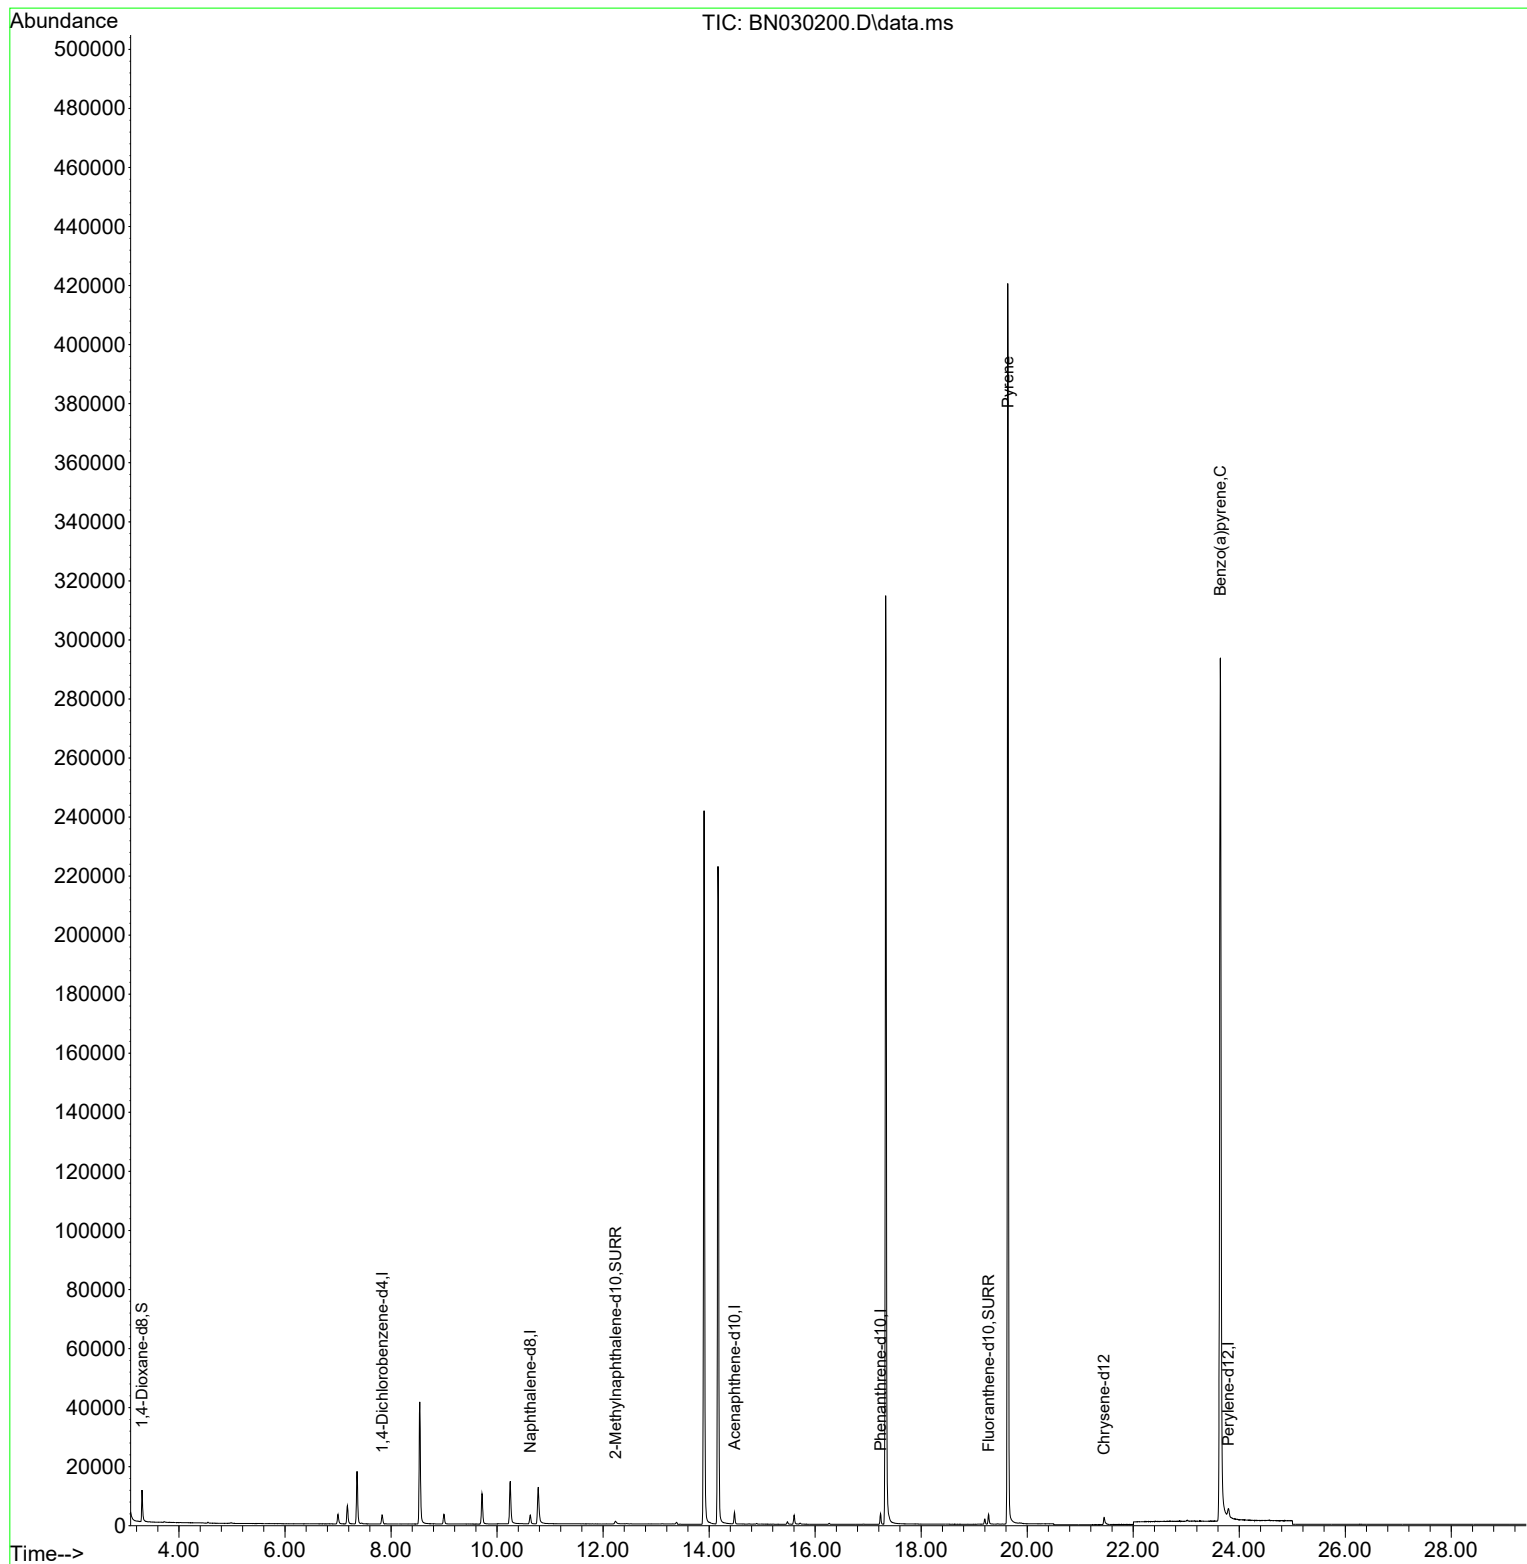

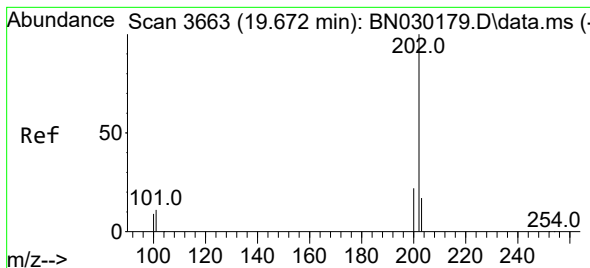

#20

Pyrene

Concen: 0.044 ng/ul

RT: 19.634 min Scan# 30

Delta R.T. -0.038 min

Lab File: BN030200.D

Acq: 03 Mar 2024 03:09

Instrument :

BNA_N

ClientSampleId :

E10A2





Tgt Ion:202 Resp: 727

Ion Ratio Lower Upper

202 100

101 222.0 10.6 15.8#

100 1753.8 8.8 13.2#

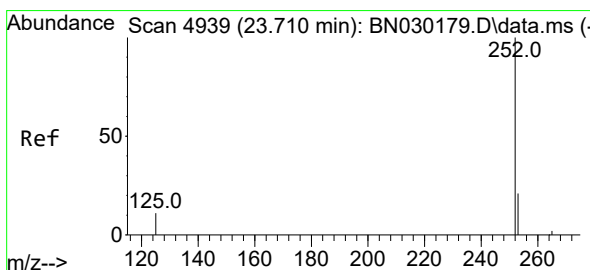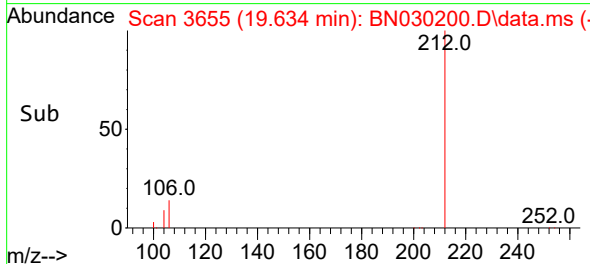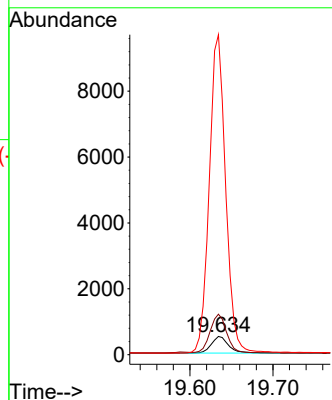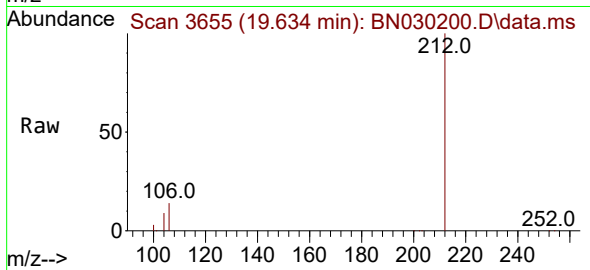

#26

Benzo(a)pyrene

Concen: 0.076 ng/ul

RT: 23.642 min Scan# 4916

Delta R.T. -0.068 min

Lab File: BN030200.D

Acq: 03 Mar 2024 03:09

Tgt Ion:252 Resp: 1686

Ion Ratio Lower Upper

252 100

253 62.9 33.0 49.4#

125 43.0 16.9 25.3#

