

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
 Data File : BN030201.D
 Acq On : 03 Mar 2024 03:45
 Operator : MA/JU
 Sample : P1501-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1098

Quant Time: Mar 03 22:50:22 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 02 16:09:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.834	152	1673	0.400	ng/ul	0.00
4) Naphthalene-d8	10.627	136	4396	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.477	164	2152	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.233	188	4160	0.400	ng/ul	#-0.01
17) Chrysene-d12	21.450	240	3031	0.400	ng/ul	# 0.00
23) Perylene-d12	23.794	264	5061	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.302	96	8572	3.701	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.233	152	1815	0.319	ng/ul	0.00
18) Fluoranthene-d10	19.271	212	3921	0.397	ng/ul	-0.01
Target Compounds						
					Qvalue	
20) Pyrene	19.638	202	721	0.049	ng/ul#	1
26) Benzo(a)pyrene	23.642	252	1618	0.081	ng/ul#	55


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
Data File : BN030201.D
Acq On : 03 Mar 2024 03:45
Operator : MA/JU
Sample : P1501-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1098

Quant Time: Mar 03 22:50:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 02 16:09:30 2024
Response via : Initial Calibration

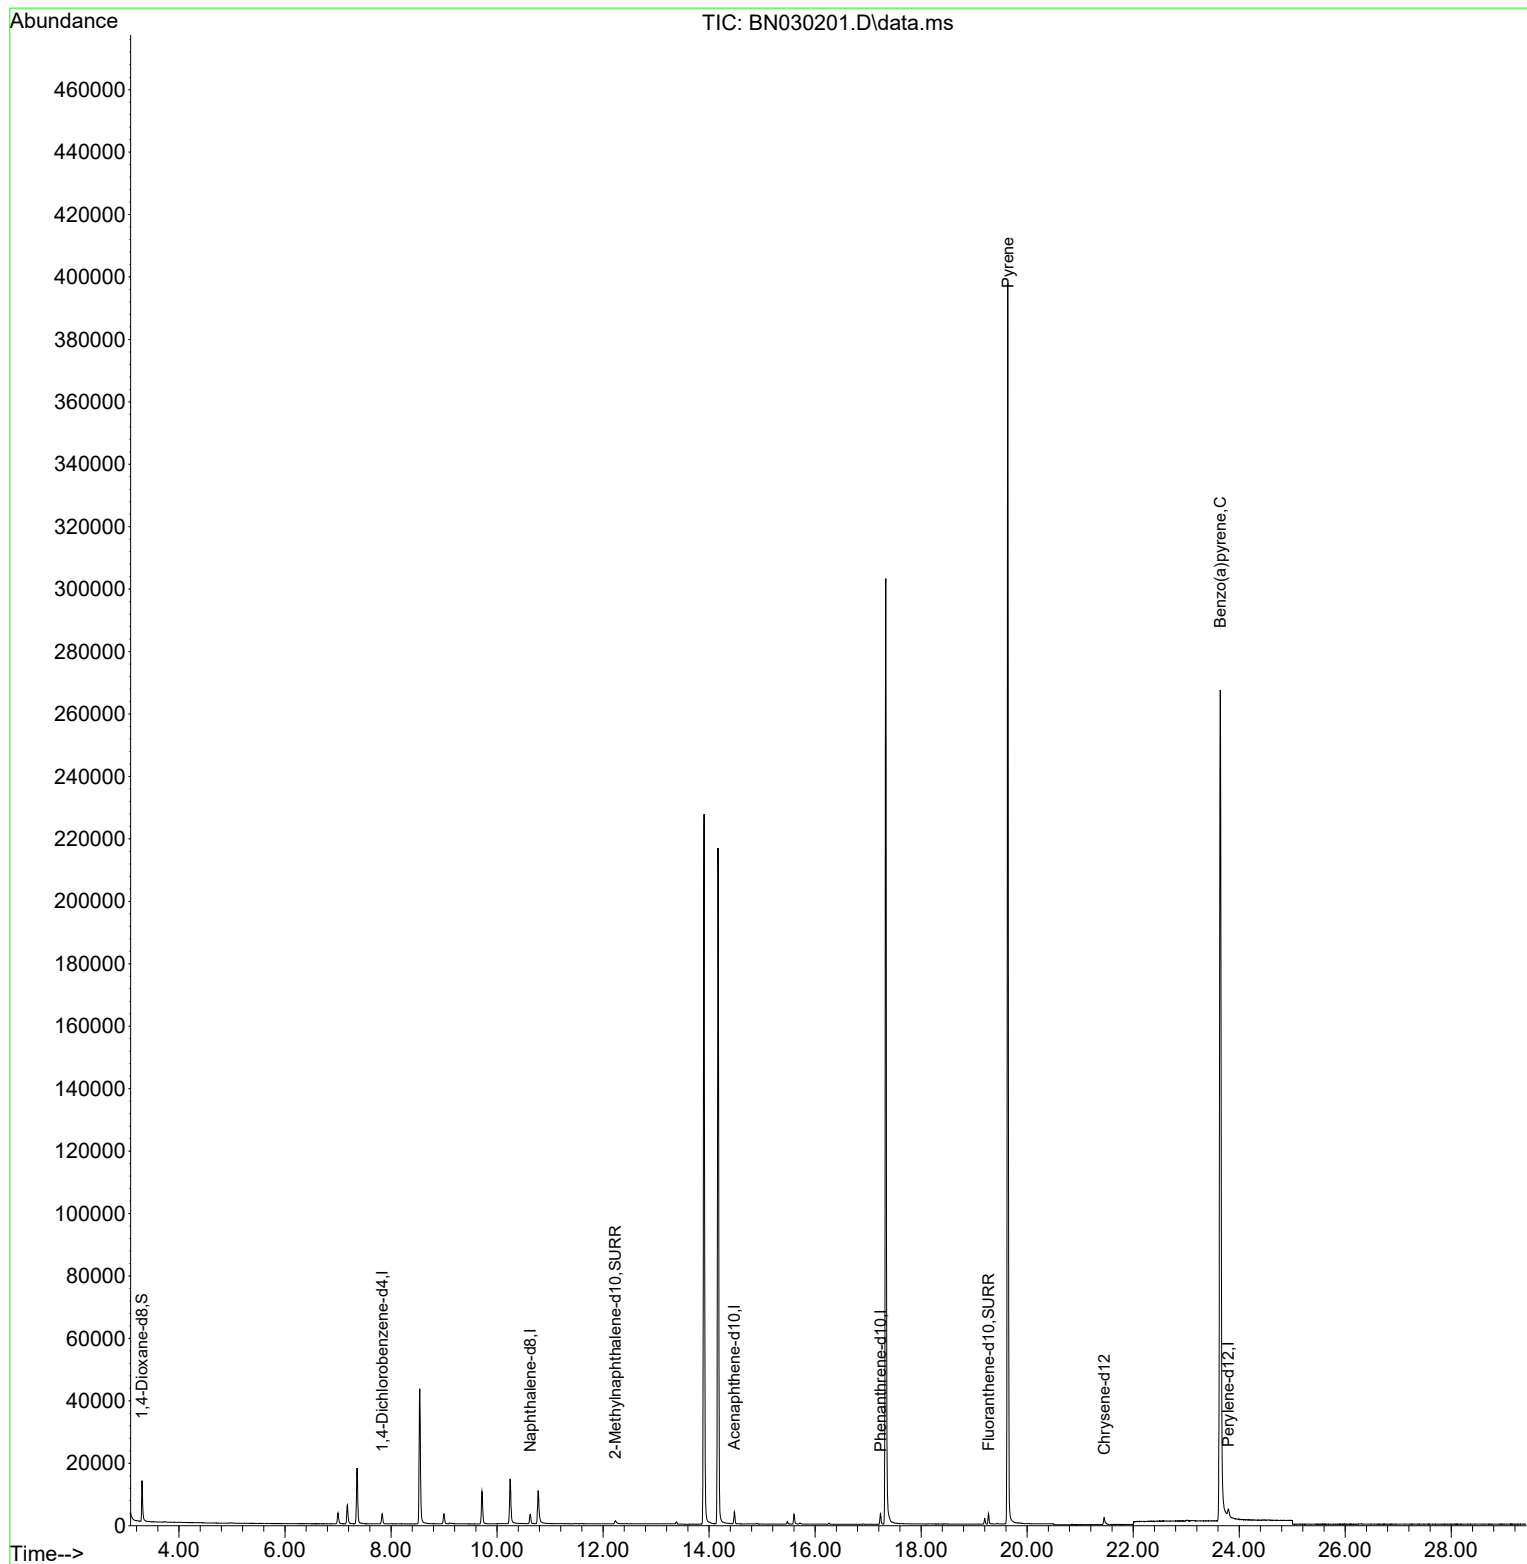

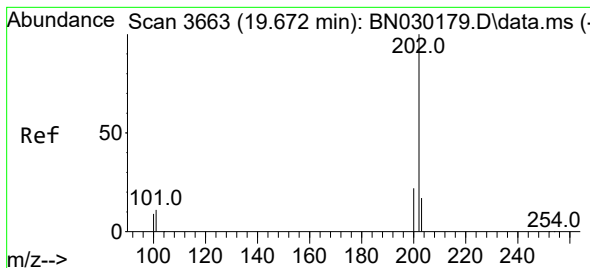

#20

Pyrene

Concen: 0.049 ng/ul

RT: 19.638 min Scan# 30

Delta R.T. -0.035 min

Lab File: BN030201.D

Acq: 03 Mar 2024 03:45

Instrument :

BNA_N

ClientSampleId :

E1098





Tgt Ion:202 Resp: 721

Ion Ratio Lower Upper

202 100

101 216.3 10.6 15.8#

100 1570.2 8.8 13.2#

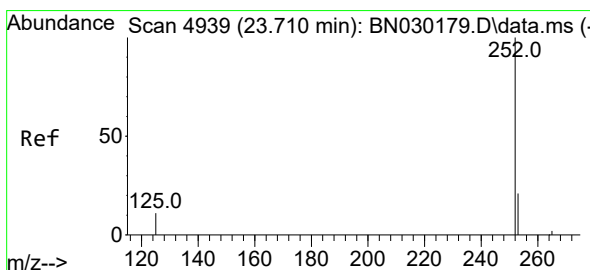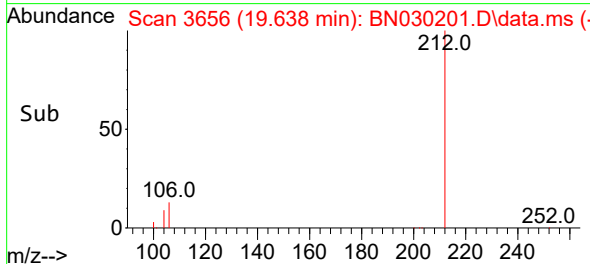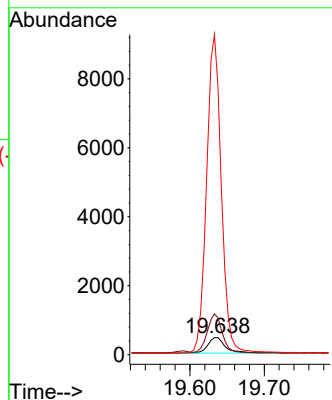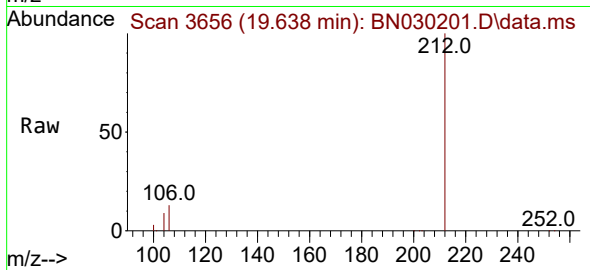

#26

Benzo(a)pyrene

Concen: 0.081 ng/ul

RT: 23.642 min Scan# 4916

Delta R.T. -0.068 min

Lab File: BN030201.D

Acq: 03 Mar 2024 03:45

Tgt Ion:252 Resp: 1618

Ion Ratio Lower Upper

252 100

253 66.4 33.0 49.4#

125 46.8 16.9 25.3#

