

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
 Data File : BN030207.D
 Acq On : 03 Mar 2024 07:58
 Operator : MA/JU
 Sample : PB159246BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK246

Quant Time: Mar 03 22:51:19 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 02 16:09:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.830	152	1886	0.400	ng/ul	0.00
4) Naphthalene-d8	10.623	136	4882	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.479	164	2457	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.234	188	4807	0.400	ng/ul	#-0.01
17) Chrysene-d12	21.453	240	3425	0.400	ng/ul	# 0.00
23) Perylene-d12	23.794	264	5761	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.302	96	11091	4.248	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.229	152	1660	0.263	ng/ul	-0.01
18) Fluoranthene-d10	19.272	212	3198	0.287	ng/ul	-0.01
Target Compounds						
					Qvalue	
12) Fluorene	15.473	166	613	0.060	ng/ul#	19
20) Pyrene	19.634	202	561	0.034	ng/ul#	1
26) Benzo(a)pyrene	23.642	252	1387	0.061	ng/ul#	49


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
Data File : BN030207.D
Acq On : 03 Mar 2024 07:58
Operator : MA/JU
Sample : PB159246BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK246

Quant Time: Mar 03 22:51:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 02 16:09:30 2024
Response via : Initial Calibration




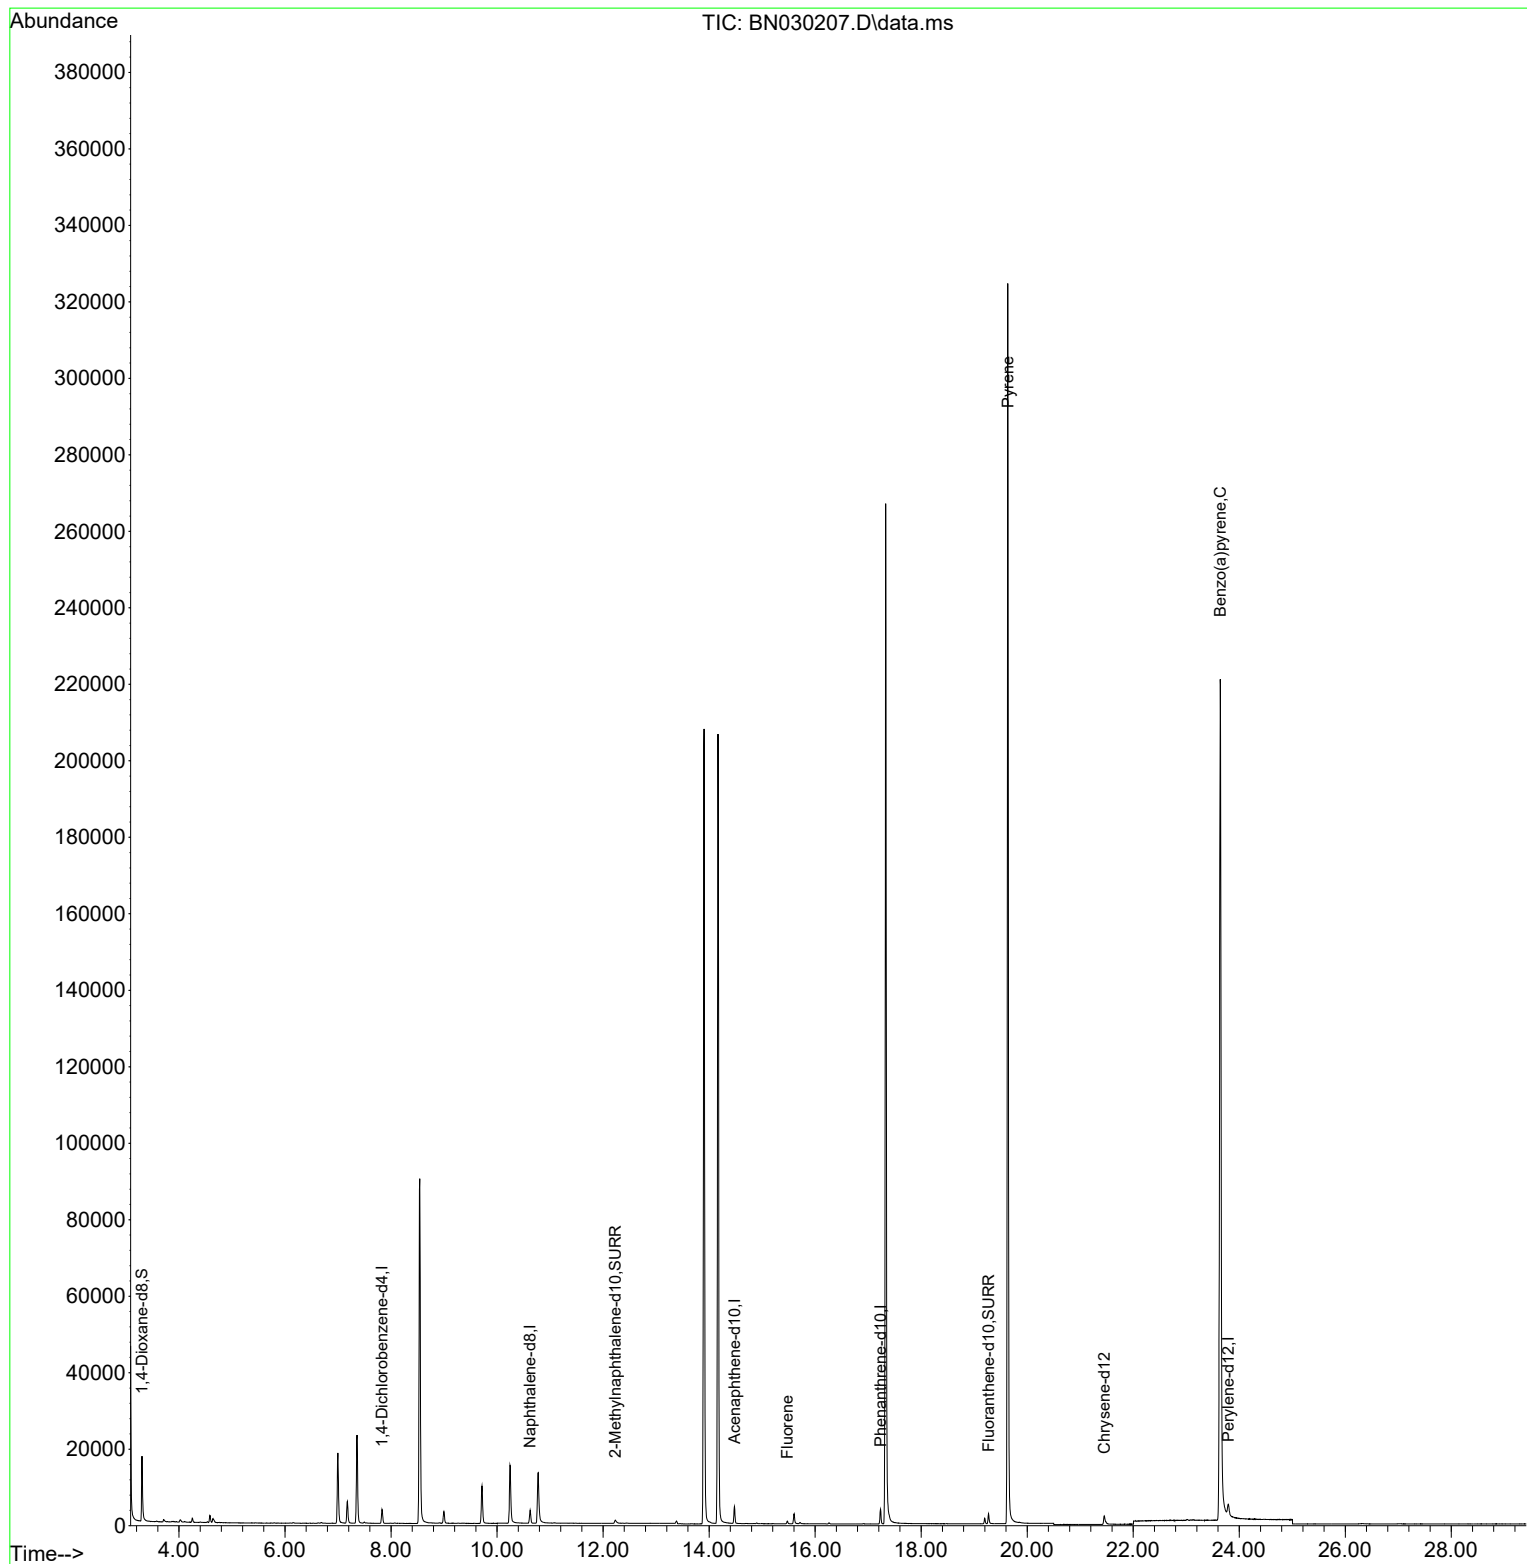


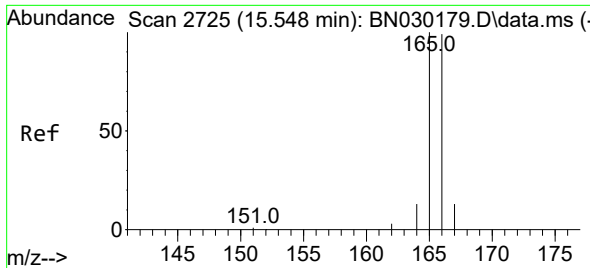

#12
Fluorene
Concen: 0.060 ng/ul
RT: 15.473 min Scan# 21
Delta R.T. -0.075 min
Lab File: BN030207.D
Acq: 03 Mar 2024 07:58




Instrument :
BNA_N
ClientSampleId :
SBLK246


Tgt Ion:166 Resp: 613
Ion Ratio Lower Upper
166 100
165 14.6 81.8 122.6#
167 37.3 13.0 19.4#

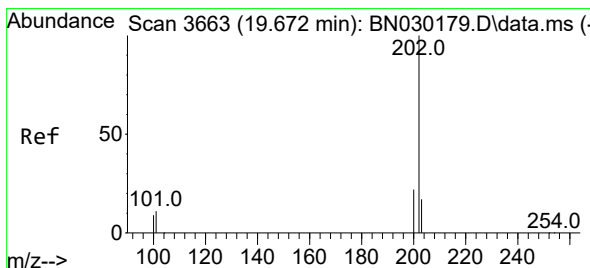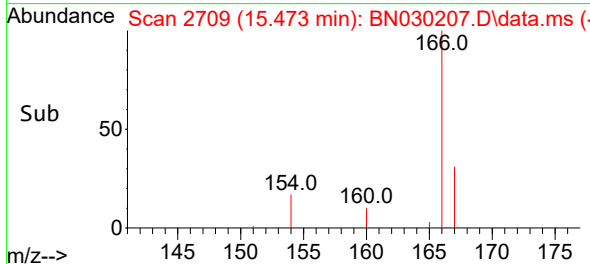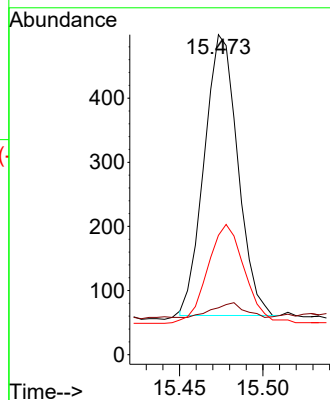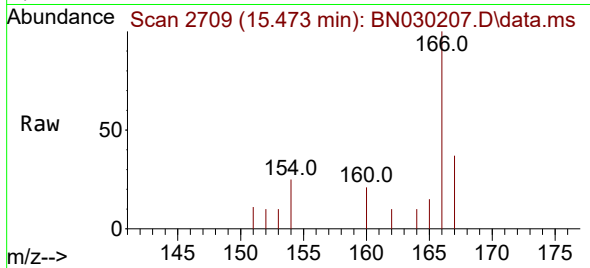

#20
Pyrene
Concen: 0.034 ng/ul
RT: 19.634 min Scan# 3655
Delta R.T. -0.038 min
Lab File: BN030207.D
Acq: 03 Mar 2024 07:58


Tgt Ion:202 Resp: 561
Ion Ratio Lower Upper
202 100
101 229.9 10.6 15.8#
100 1737.9 8.8 13.2#

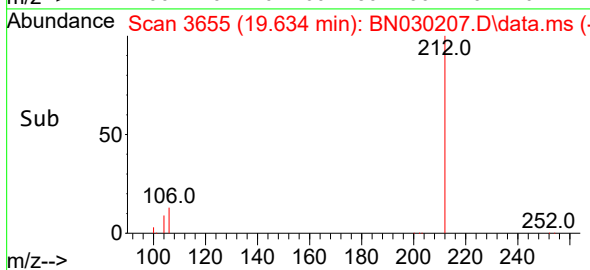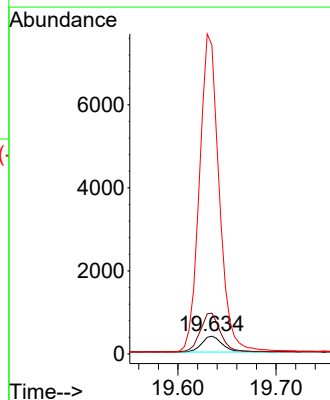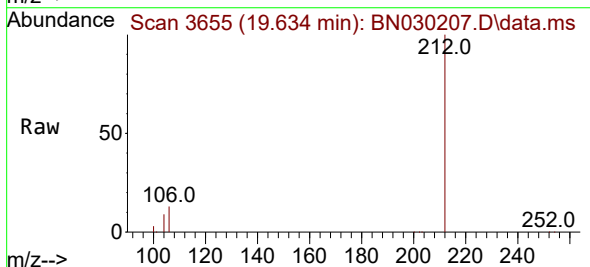

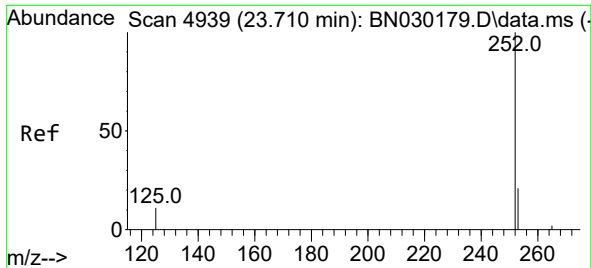

#26
Benzo(a)pyrene
Concen: 0.061 ng/ul
RT: 23.642 min Scan# 4916
Delta R.T. -0.068 min
Lab File: BN030207.D
Acq: 03 Mar 2024 07:58

Instrument :
BNA_N
ClientSampleId :
SBLK246

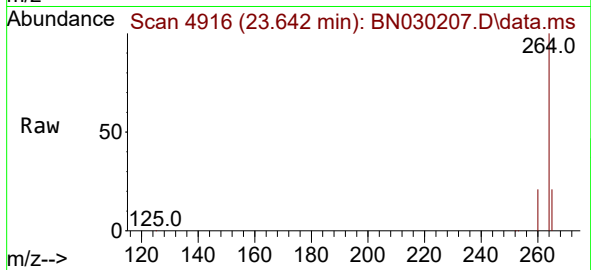

Tgt Ion:252 Resp: 1387
Ion Ratio Lower Upper
252 100
253 71.5 33.0 49.4#
125 47.4 16.9 25.3#

