

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
 Data File : BN030218.D
 Acq On : 03 Mar 2024 14:34
 Operator : MA/JU
 Sample : P1512-07
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E0SA5

Quant Time: Mar 03 22:53:16 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 02 16:09:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.829	152	1884	0.400	ng/ul	0.00
4) Naphthalene-d8	10.623	136	4884	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.479	164	2322	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.234	188	4562	0.400	ng/ul	#-0.01
17) Chrysene-d12	21.447	240	3814	0.400	ng/ul	# 0.00
23) Perylene-d12	23.794	264	5697	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.302	96	11618	4.454	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.223	152	1826	0.289	ng/ul	-0.02
18) Fluoranthene-d10	19.272	212	3459	0.278	ng/ul	-0.01
Target Compounds						
					Qvalue	
20) Pyrene	19.634	202	699	0.038	ng/ul#	1
26) Benzo(a)pyrene	23.645	252	1558	0.070	ng/ul#	41


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
Data File : BN030218.D
Acq On : 03 Mar 2024 14:34
Operator : MA/JU
Sample : P1512-07
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0SA5

Quant Time: Mar 03 22:53:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 02 16:09:30 2024
Response via : Initial Calibration

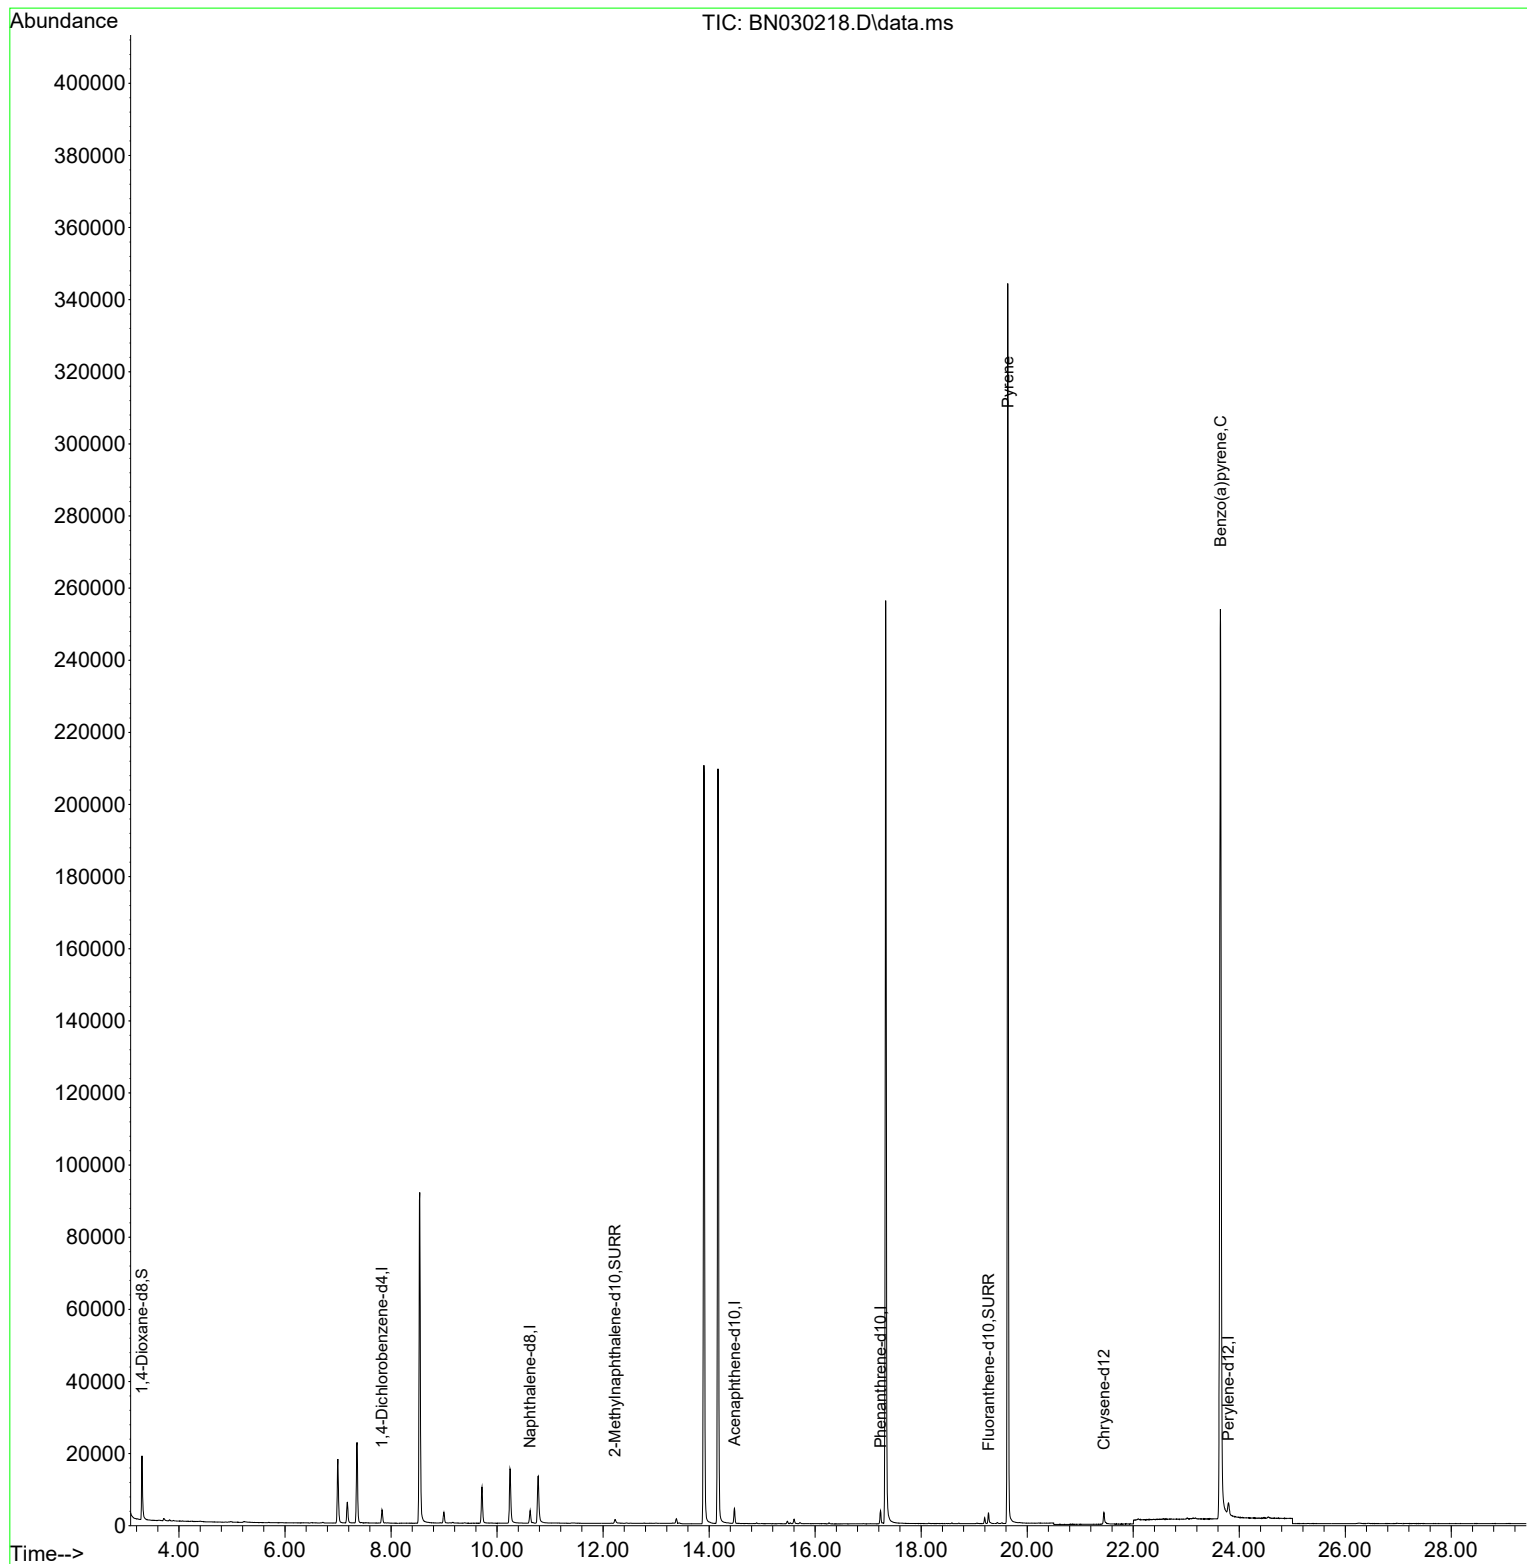

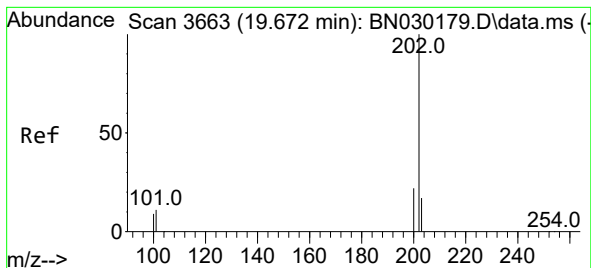

#20

Pyrene

Concen: 0.038 ng/ul

RT: 19.634 min Scan# 3

Delta R.T. -0.038 min

Lab File: BN030218.D

Acq: 03 Mar 2024 14:34

Instrument :

BNA_N

ClientSampleId :

E0SA5





Tgt Ion:202 Resp: 699

Ion Ratio Lower Upper

202 100

101 213.6 10.6 15.8#

100 1628.6 8.8 13.2#

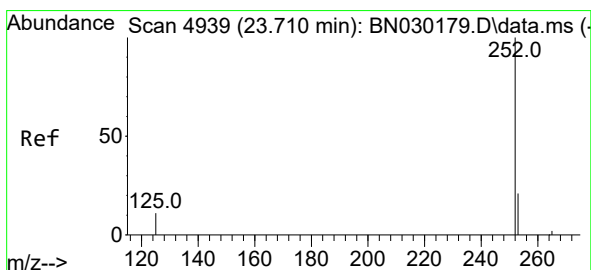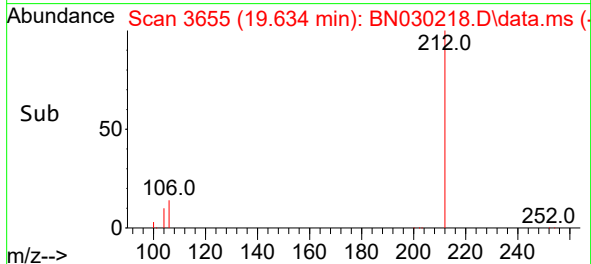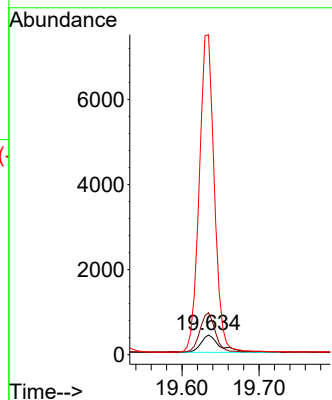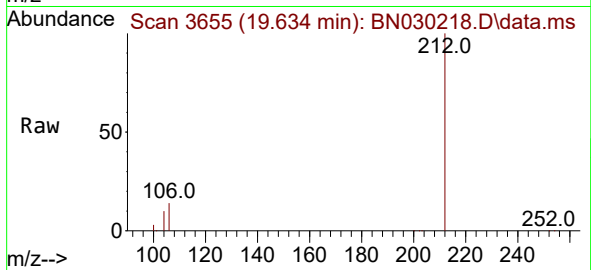

#26

Benzo(a)pyrene

Concen: 0.070 ng/ul

RT: 23.645 min Scan# 4917

Delta R.T. -0.065 min

Lab File: BN030218.D

Acq: 03 Mar 2024 14:34

Tgt Ion:252 Resp: 1558

Ion Ratio Lower Upper

252 100

253 77.6 33.0 49.4#

125 49.2 16.9 25.3#

