

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
 Data File : BN030224.D
 Acq On : 03 Mar 2024 18:47
 Operator : MA/JU
 Sample : PB159151BL
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK151

Quant Time: Mar 03 22:54:27 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 02 16:09:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.830	152	1352	0.400	ng/ul	0.00
4) Naphthalene-d8	10.623	136	3554	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.474	164	1762	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.230	188	3483	0.400	ng/ul	#-0.02
17) Chrysene-d12	21.453	240	2785	0.400	ng/ul	0.00
23) Perylene-d12	23.791	264	5154	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.302	96	10660	5.695	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.229	152	1443	0.314	ng/ul	-0.01
18) Fluoranthene-d10	19.272	212	2739	0.302	ng/ul	-0.01
Target Compounds						
					Qvalue	
12) Fluorene	15.473	166	524	0.071	ng/ul#	21
20) Pyrene	19.634	202	500	0.037	ng/ul#	1
26) Benzo(a)pyrene	23.648	252	1345	0.066	ng/ul#	51


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
Data File : BN030224.D
Acq On : 03 Mar 2024 18:47
Operator : MA/JU
Sample : PB159151BL
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK151

Quant Time: Mar 03 22:54:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 02 16:09:30 2024
Response via : Initial Calibration




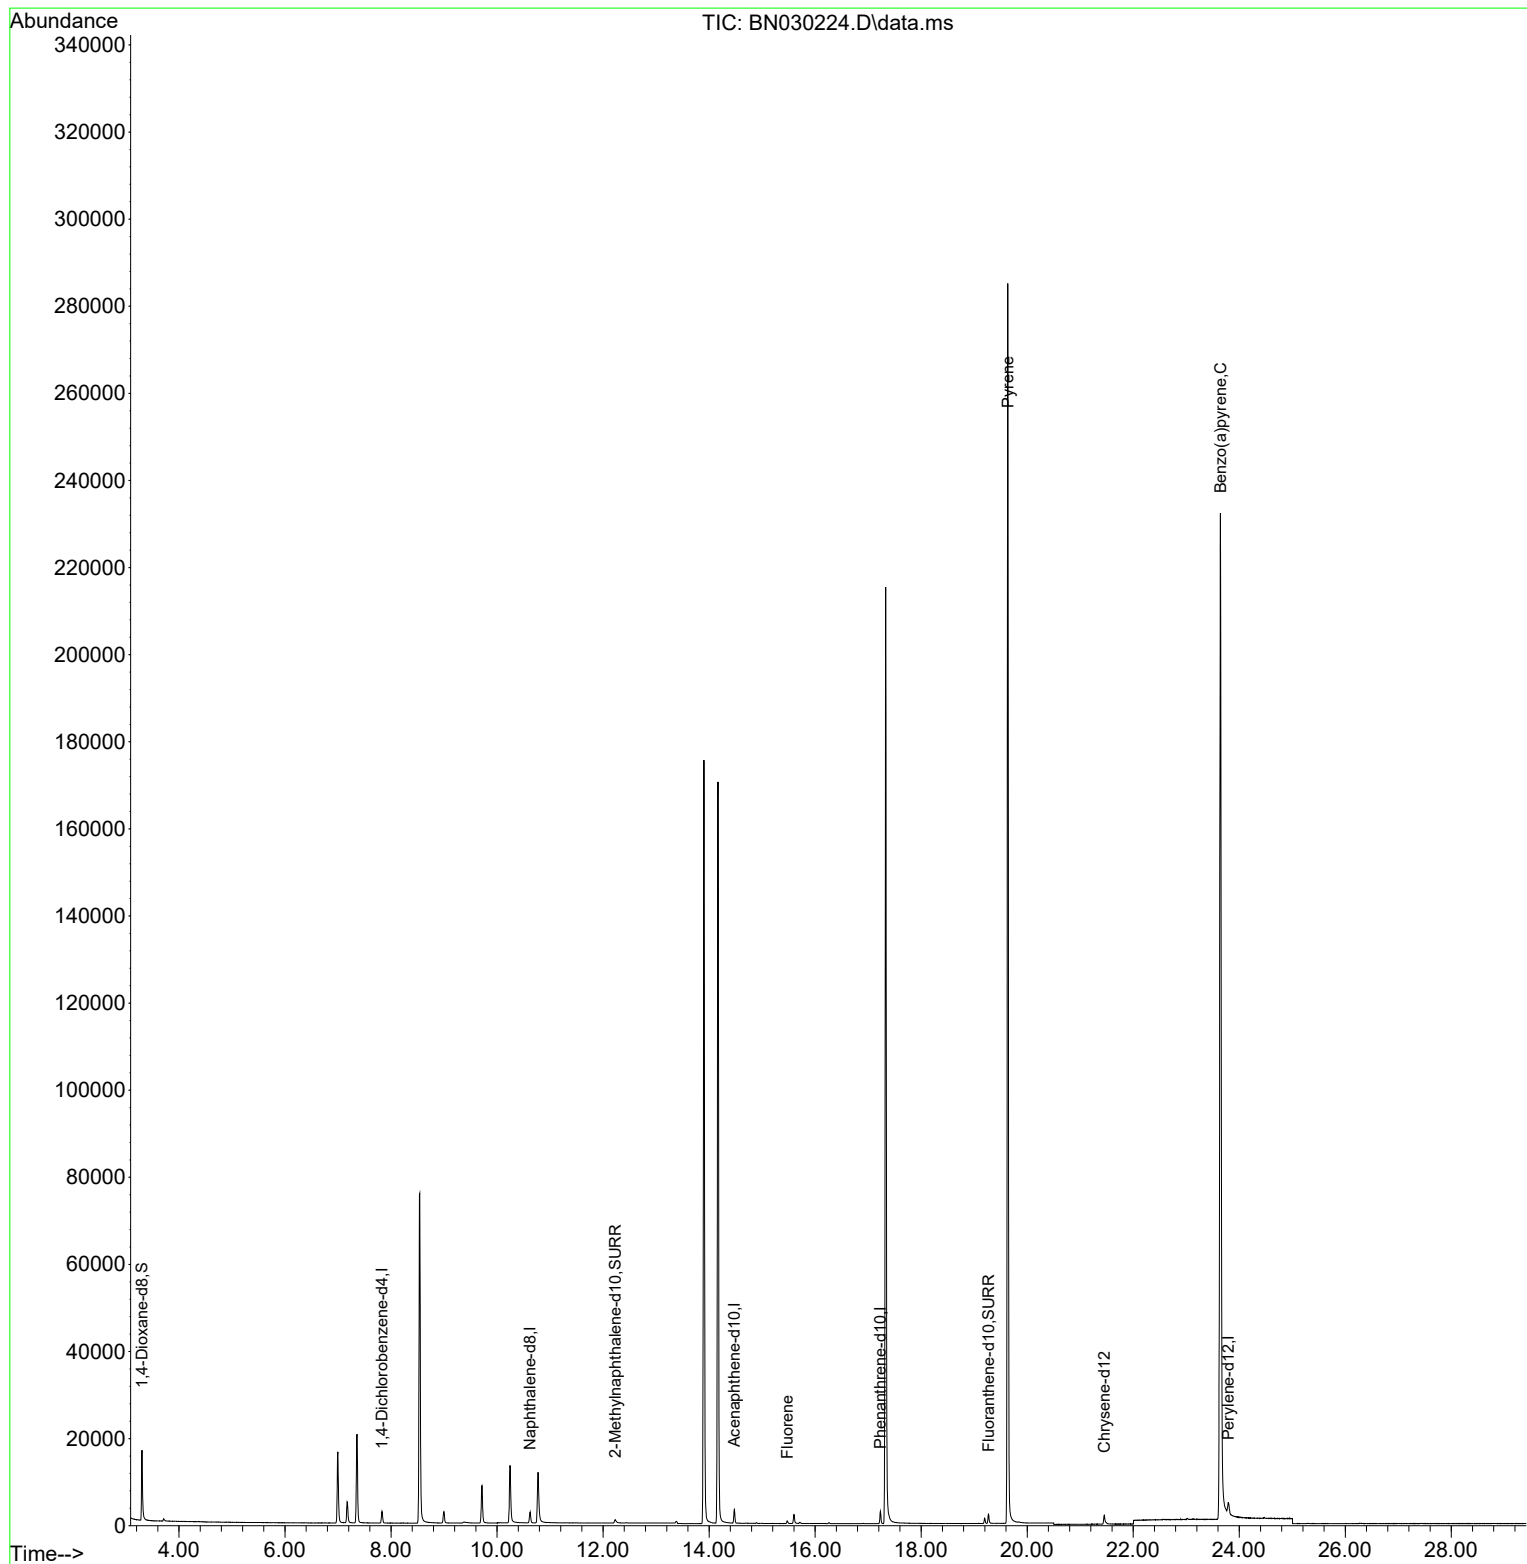


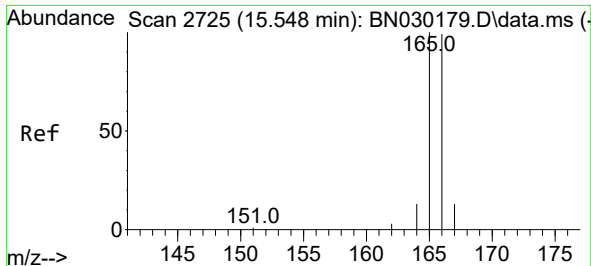

#12
Fluorene
Concen: 0.071 ng/ul
RT: 15.473 min Scan# 21
Delta R.T. -0.075 min
Lab File: BN030224.D
Acq: 03 Mar 2024 18:47




Instrument :
BNA_N
ClientSampleId :
SBLK151


Tgt Ion:166 Resp: 524
Ion Ratio Lower Upper
166 100
165 18.1 81.8 122.6#
167 40.3 13.0 19.4#

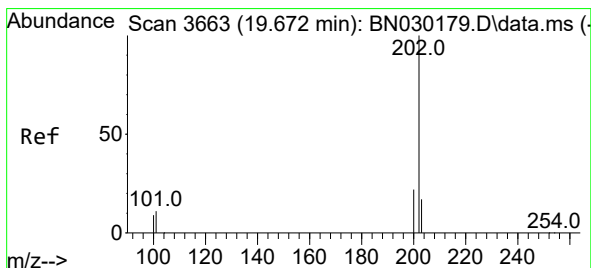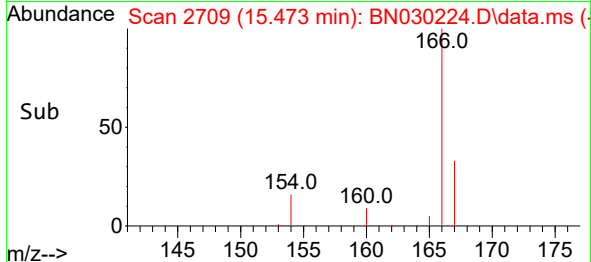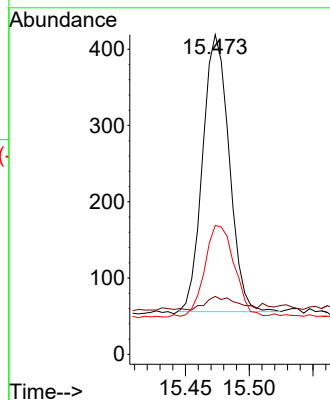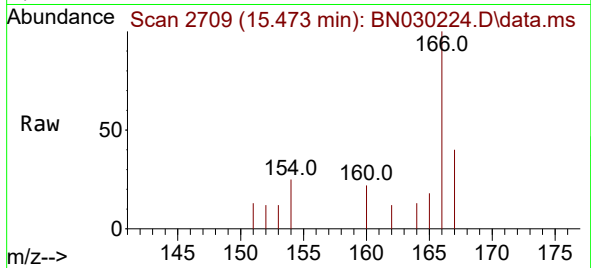

#20
Pyrene
Concen: 0.037 ng/ul
RT: 19.634 min Scan# 3655
Delta R.T. -0.038 min
Lab File: BN030224.D
Acq: 03 Mar 2024 18:47


Tgt Ion:202 Resp: 500
Ion Ratio Lower Upper
202 100
101 219.0 10.6 15.8#
100 1638.5 8.8 13.2#

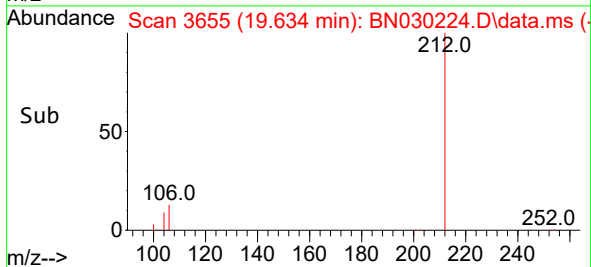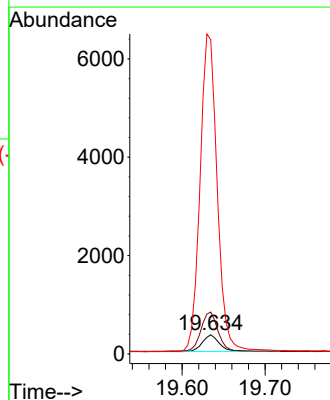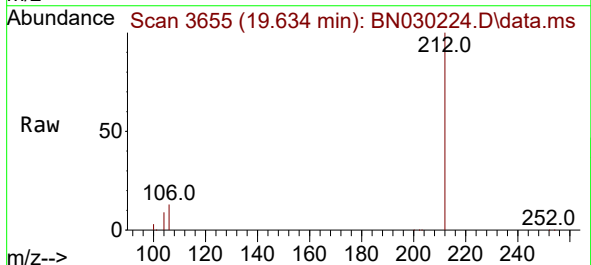

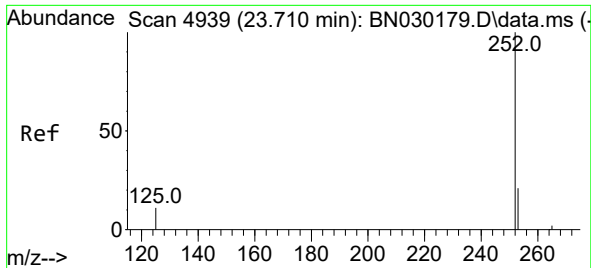

#26
Benzo(a)pyrene
Concen: 0.066 ng/ul
RT: 23.648 min Scan# 4918
Delta R.T. -0.062 min
Lab File: BN030224.D
Acq: 03 Mar 2024 18:47

Instrument :
BNA_N
ClientSampleId :
SBLK151

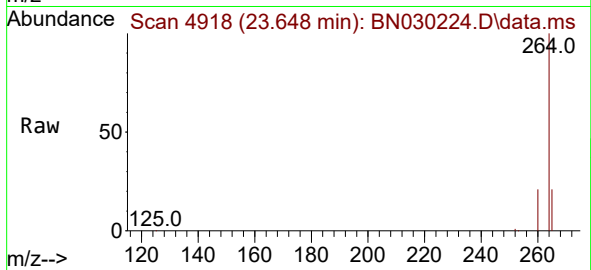

Tgt Ion:252 Resp: 1345
Ion Ratio Lower Upper
252 100
253 70.3 33.0 49.4#
125 46.0 16.9 25.3#

