

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
 Data File : BN030225.D
 Acq On : 03 Mar 2024 19:23
 Operator : MA/JU
 Sample : PB159243BL
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK243

Quant Time: Mar 03 22:54:34 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 02 16:09:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.829	152	1510	0.400	ng/ul	0.00
4) Naphthalene-d8	10.623	136	4005	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.475	164	1989	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.231	188	3850	0.400	ng/ul	#-0.02
17) Chrysene-d12	21.451	240	2945	0.400	ng/ul	# 0.00
23) Perylene-d12	23.792	264	5159	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.302	96	12928	6.184	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.228	152	1708	0.330	ng/ul	-0.01
18) Fluoranthene-d10	19.268	212	3178	0.331	ng/ul	-0.01
Target Compounds						Qvalue
12) Fluorene	15.474	166	614	0.074	ng/ul#	21
20) Pyrene	19.635	202	552	0.039	ng/ul#	1
26) Benzo(a)pyrene	23.643	252	1534	0.076	ng/ul#	53


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
Data File : BN030225.D
Acq On : 03 Mar 2024 19:23
Operator : MA/JU
Sample : PB159243BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK243

Quant Time: Mar 03 22:54:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 02 16:09:30 2024
Response via : Initial Calibration




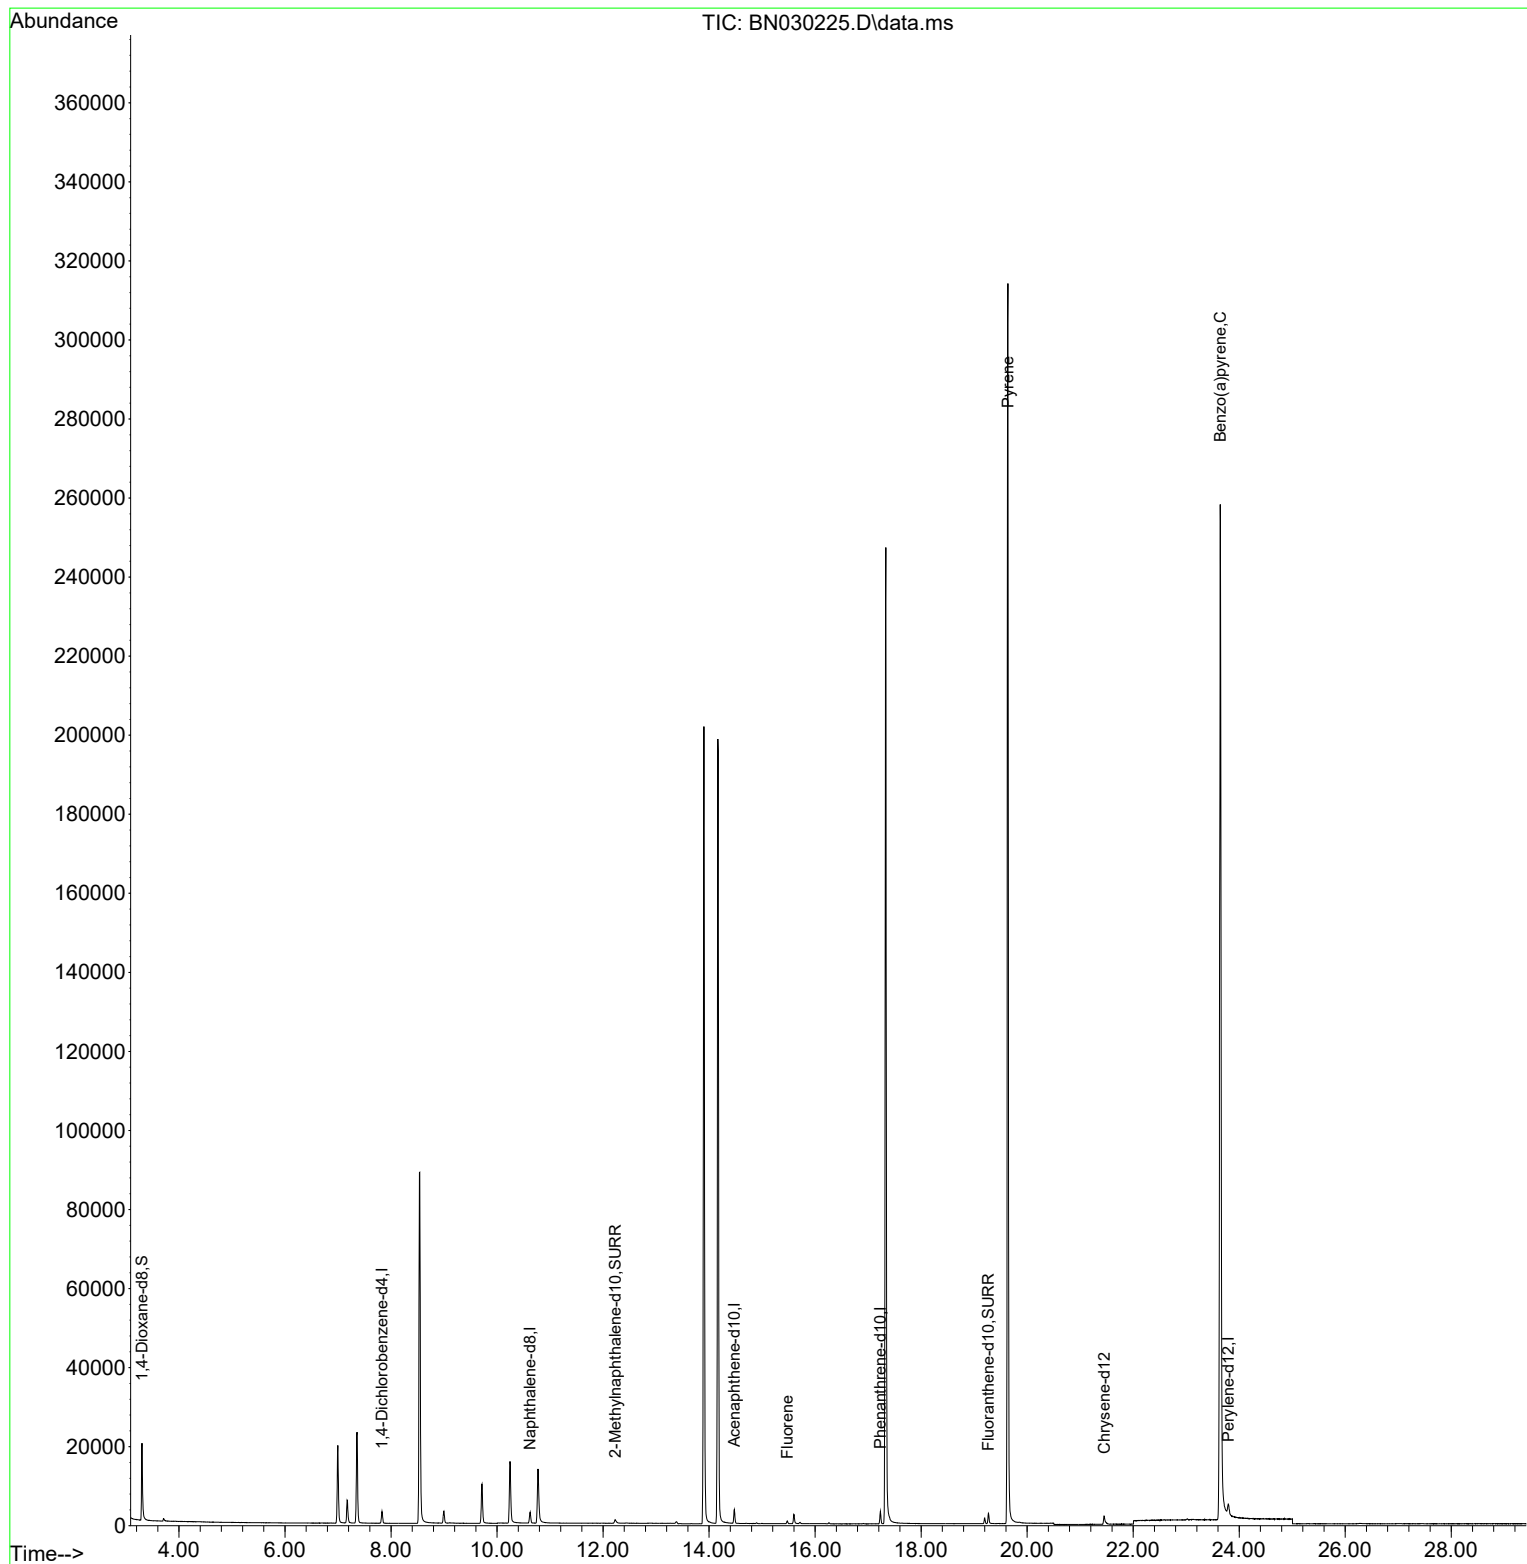


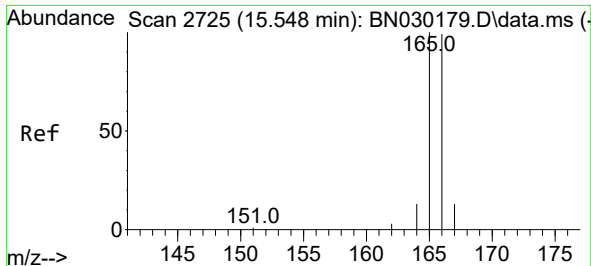

#12
Fluorene
Concen: 0.074 ng/ul
RT: 15.474 min Scan# 21
Delta R.T. -0.074 min
Lab File: BN030225.D
Acq: 03 Mar 2024 19:23




Instrument :
BNA_N
ClientSampleId :
SBLK243


Tgt Ion:166 Resp: 614
Ion Ratio Lower Upper
166 100
165 17.7 81.8 122.6#
167 39.1 13.0 19.4#

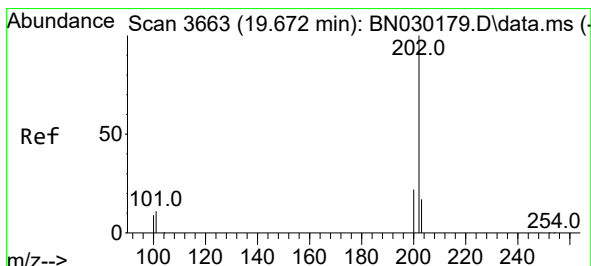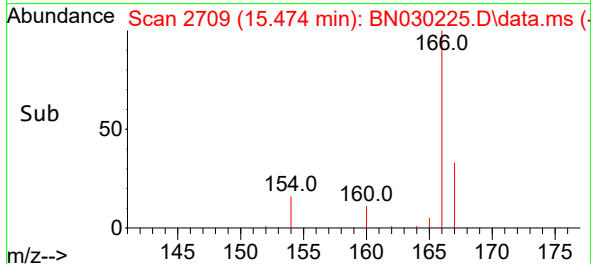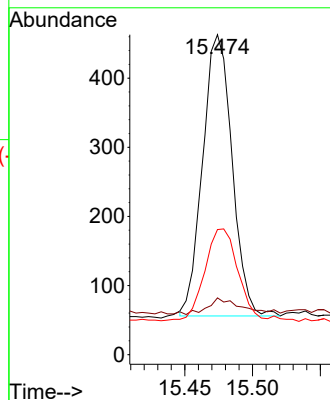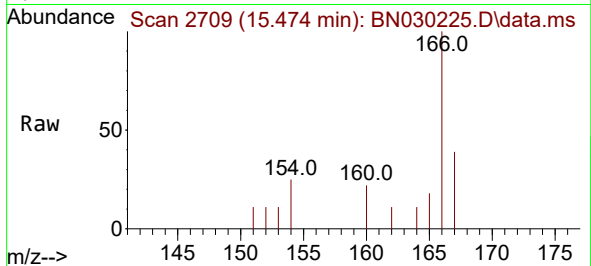

#20
Pyrene
Concen: 0.039 ng/ul
RT: 19.635 min Scan# 3655
Delta R.T. -0.037 min
Lab File: BN030225.D
Acq: 03 Mar 2024 19:23


Tgt Ion:202 Resp: 552
Ion Ratio Lower Upper
202 100
101 219.7 10.6 15.8#
100 1628.4 8.8 13.2#

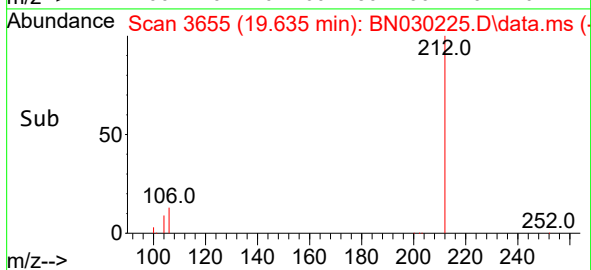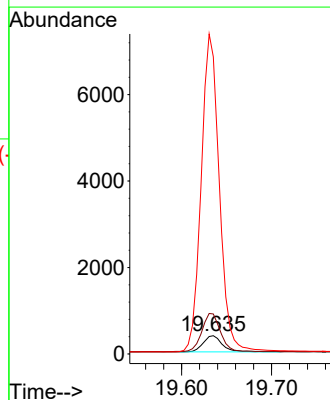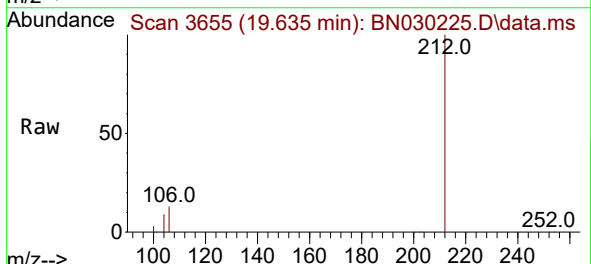

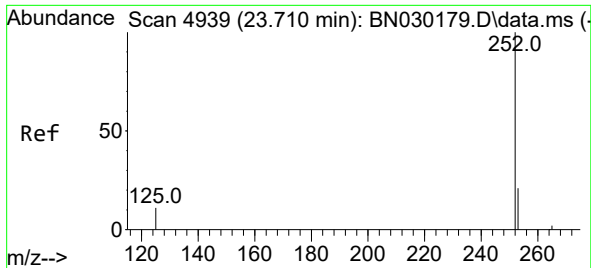

#26
Benzo(a)pyrene
Concen: 0.076 ng/ul
RT: 23.643 min Scan# 4916
Delta R.T. -0.067 min
Lab File: BN030225.D
Acq: 03 Mar 2024 19:23

Instrument :
BNA_N
ClientSampleId :
SBLK243

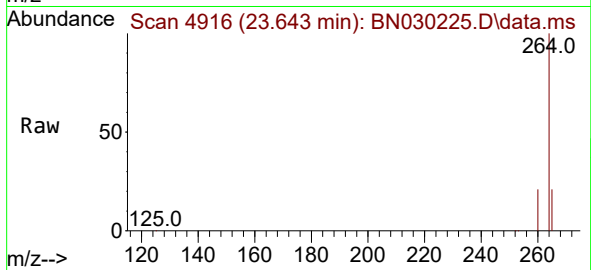

Tgt Ion:252 Resp: 1534
Ion Ratio Lower Upper
252 100
253 69.8 33.0 49.4#
125 45.1 16.9 25.3#

