

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
Data File : BN030196.D
Acq On : 03 Mar 2024 00:44
Operator : MA/JU
Sample : P1501-10
Misc :
ALS Vial : 16 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
E10B1

Manual IntegrationsAPPROVED

Quant Time: Mar 03 22:49:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 02 16:09:30 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/04/2024
Supervised By :mohammad ahmed 03/05/2024

03/04/2024
Supervised By :mohammad
ahmed

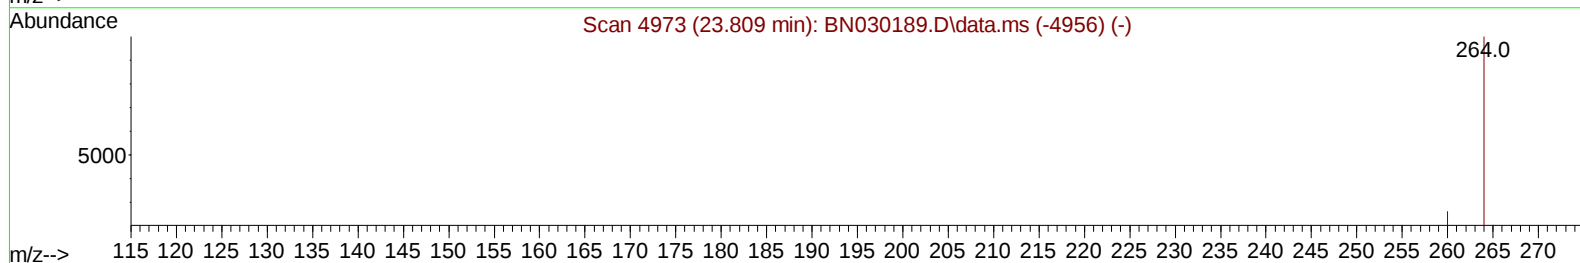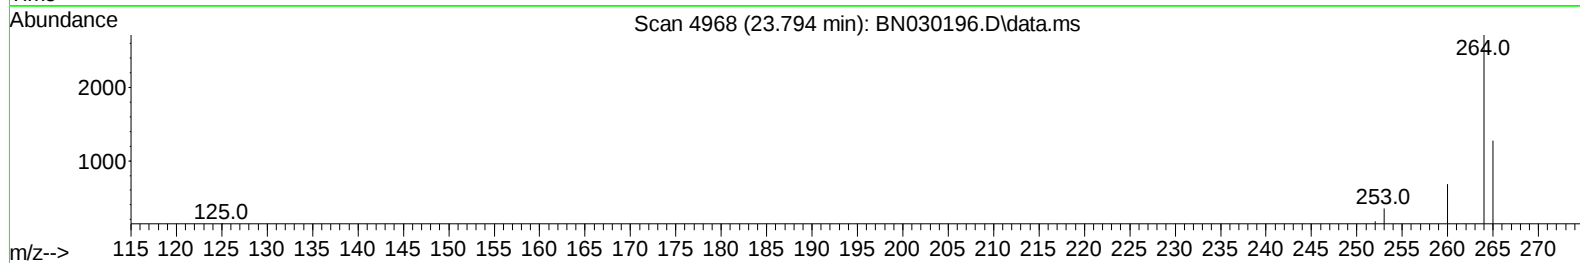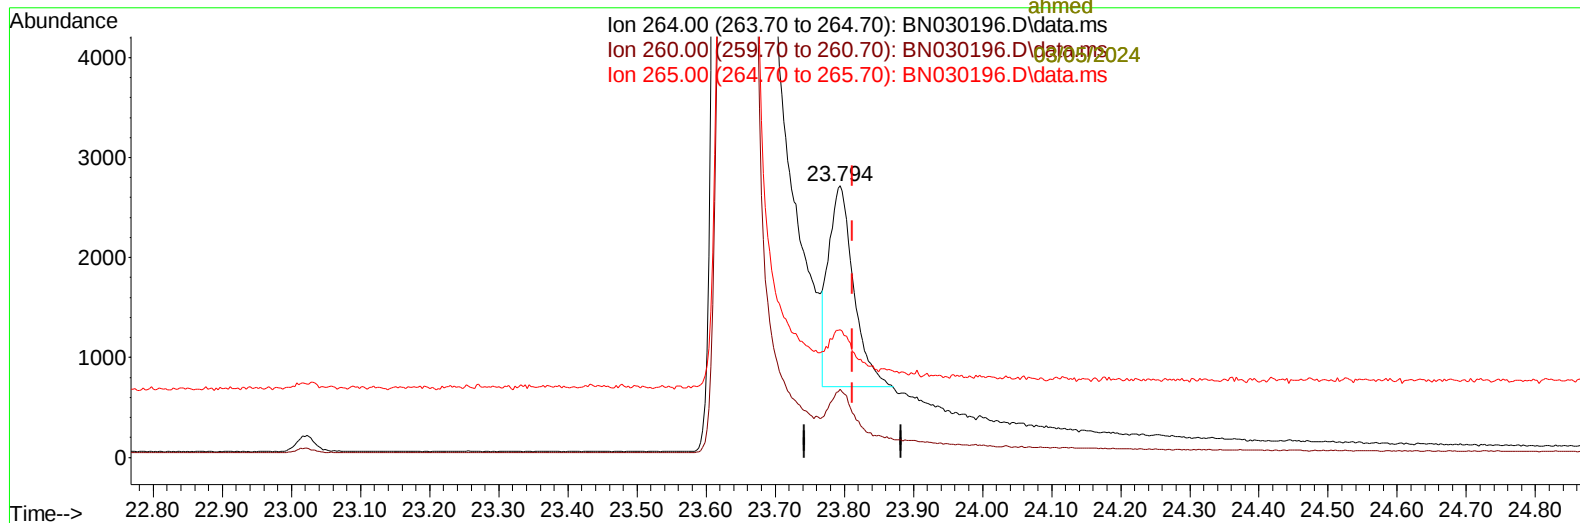

TIC: BN030196.D\data.ms

(23) Perylene-d12 (I)

23.794min (-0.018) 0.40 ng/u1

response 5085

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	29.20	25.04
265.00	110.00	46.94#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
Data File : BN030196.D
Acq On : 03 Mar 2024 00:44
Operator : MA/JU
Sample : P1501-10
Misc :
ALS Vial : 16 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
E10B1

Manual IntegrationsAPPROVED

Quant Time: Mar 03 22:49:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 02 16:09:30 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/04/2024
Supervised By :mohammad ahmed 03/05/2024

03/04/2024
Supervised By :mohammad
ahmed

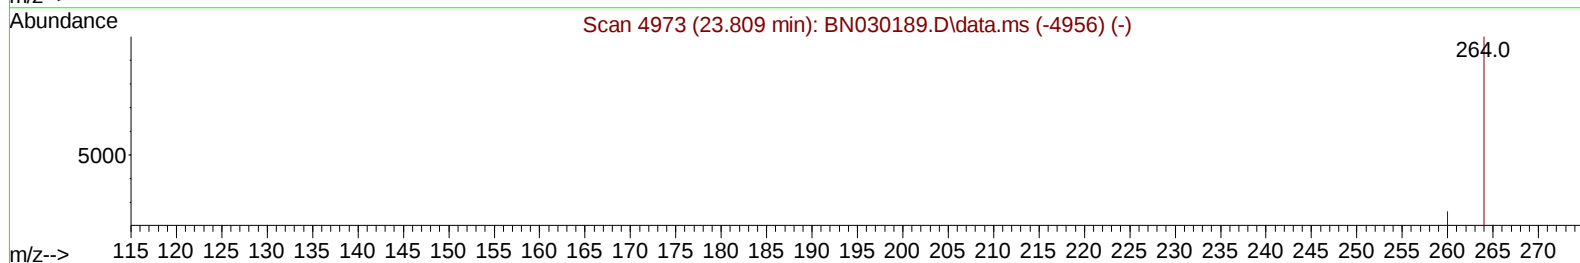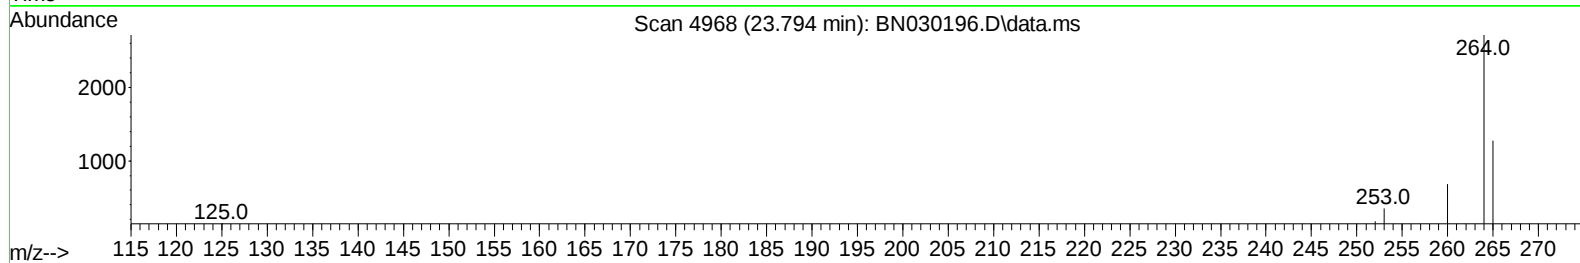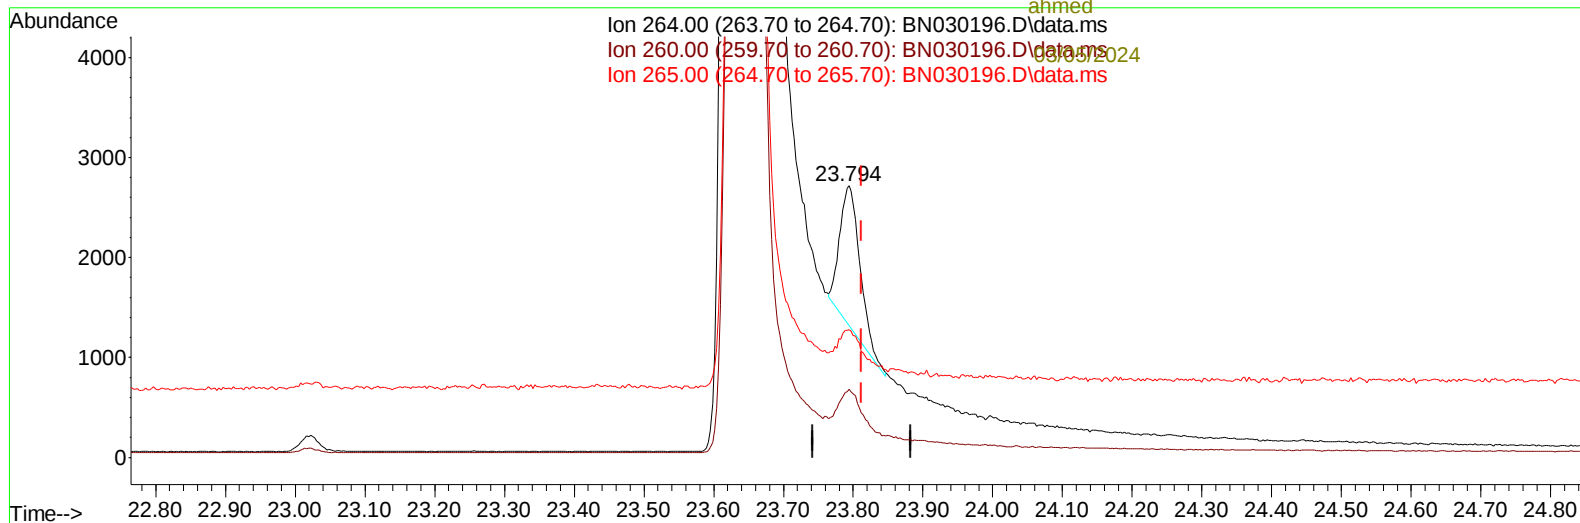

TIC: BN030196.D\data.ms

(23) Perylene-d12 (I)

23.794min (-0.018) 0.40 ng/ul m

response 2730

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	29.20	25.04
265.00	110.00	46.94#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
 Data File : BN030196.D
 Acq On : 03 Mar 2024 00:44
 Operator : MA/JU
 Sample : P1501-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E10B1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/04/2024
 Supervised By :mohammad ahmed 03/05/2024

Quant Time: Mar 03 22:49:47 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 02 16:09:30 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)
-----03/05/2024							
Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.834	152		1324	0.400	ng/ul	0.00
4) Naphthalene-d8	10.628	136		3373	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.479	164		1786	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.234	188		3627	0.400	ng/ul	#-0.01
17) Chrysene-d12	21.453	240		2827	0.400	ng/ul	0.00
23) Perylene-d12	23.794	264		2730m	0.400	ng/ul	-0.02
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.302	96		6681	3.645	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.228	152		1682	0.386	ng/ul	-0.01
18) Fluoranthene-d10	19.272	212		3824	0.415	ng/ul	-0.01
Target Compounds							
							Qvalue
5) Naphthalene	10.672	128		243	0.024	ng/ul#	50

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
Data File : BN030196.D
Acq On : 03 Mar 2024 00:44
Operator : MA/JU
Sample : P1501-10
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E10B1

Manual IntegrationsAPPROVED

Quant Time: Mar 03 22:49:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 02 16:09:30 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/04/2024
Supervised By :mohammad ahmed 03/05/2024

03/04/2024
Supervised By :mohammad
ahmed

03/05/2024

