




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
Data File : BN030197.D
Acq On : 03 Mar 2024 01:20
Operator : MA/JU
Sample : P1501-11
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E10B2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/04/2024
Supervised By :mohammad ahmed 03/05/2024

Quant Time: Mar 03 22:49:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 02 16:09:30 2024
Response via : Initial Calibration

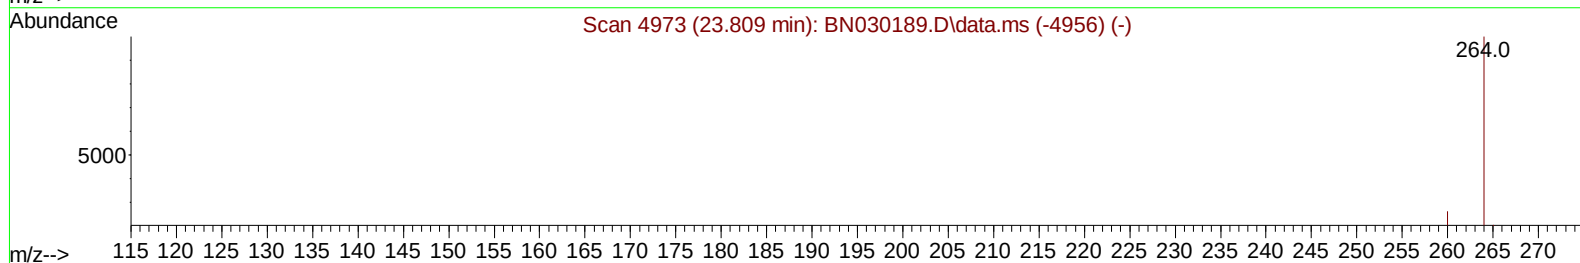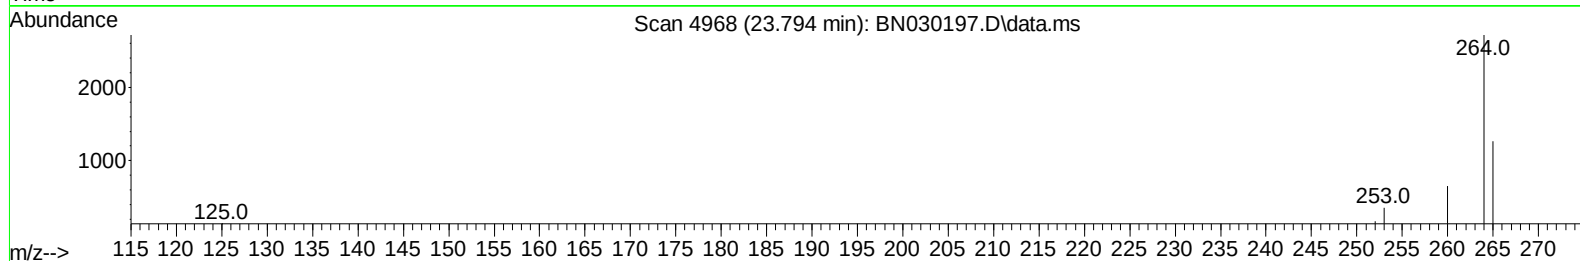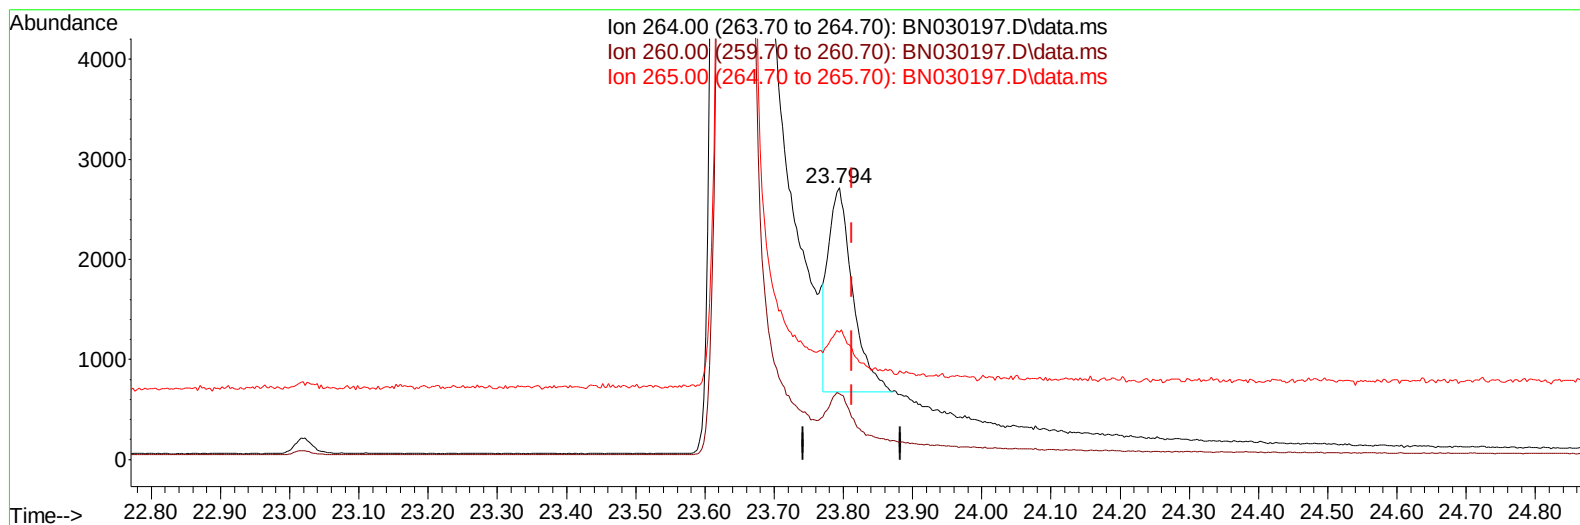

TIC: BN030197.D\data.ms

(23) Perylene-d12 (I)

23.794min (-0.018) 0.40 ng/u1

response 5004

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	29.20	24.24
265.00	110.00	46.76#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
Data File : BN030197.D
Acq On : 03 Mar 2024 01:20
Operator : MA/JU
Sample : P1501-11
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E10B2

Manual IntegrationsAPPROVED

Quant Time: Mar 03 22:49:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 02 16:09:30 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/04/2024
Supervised By :mohammad ahmed 03/05/2024

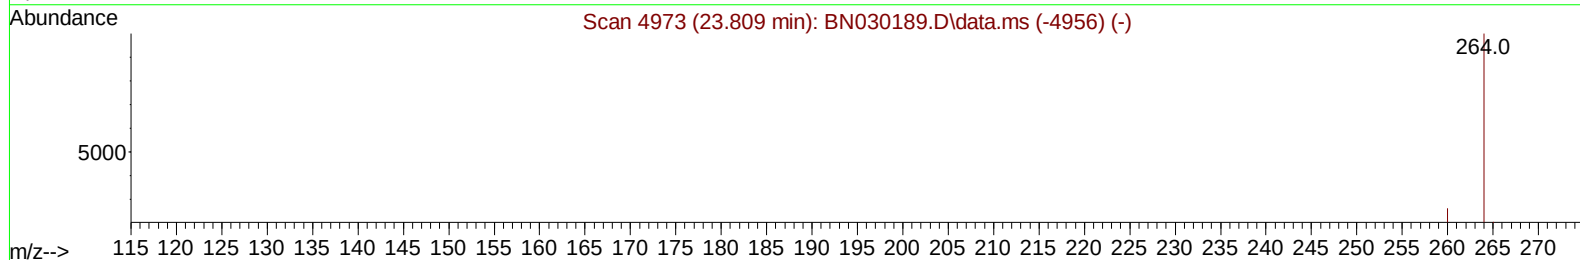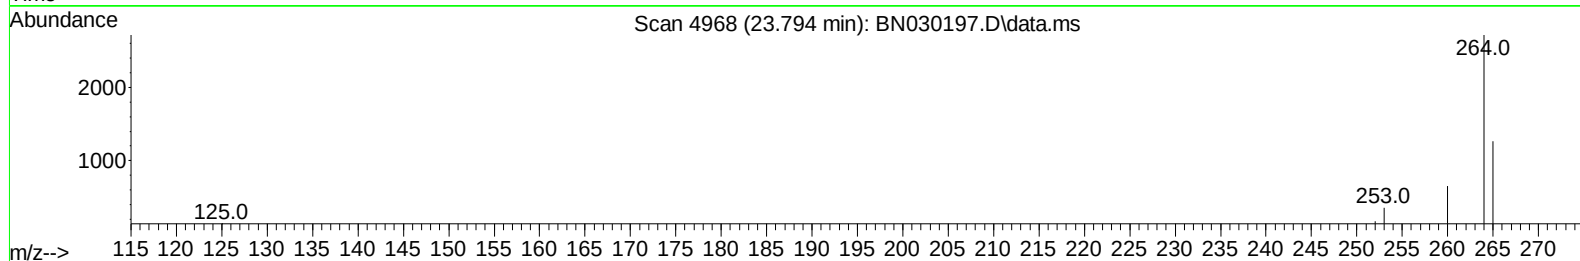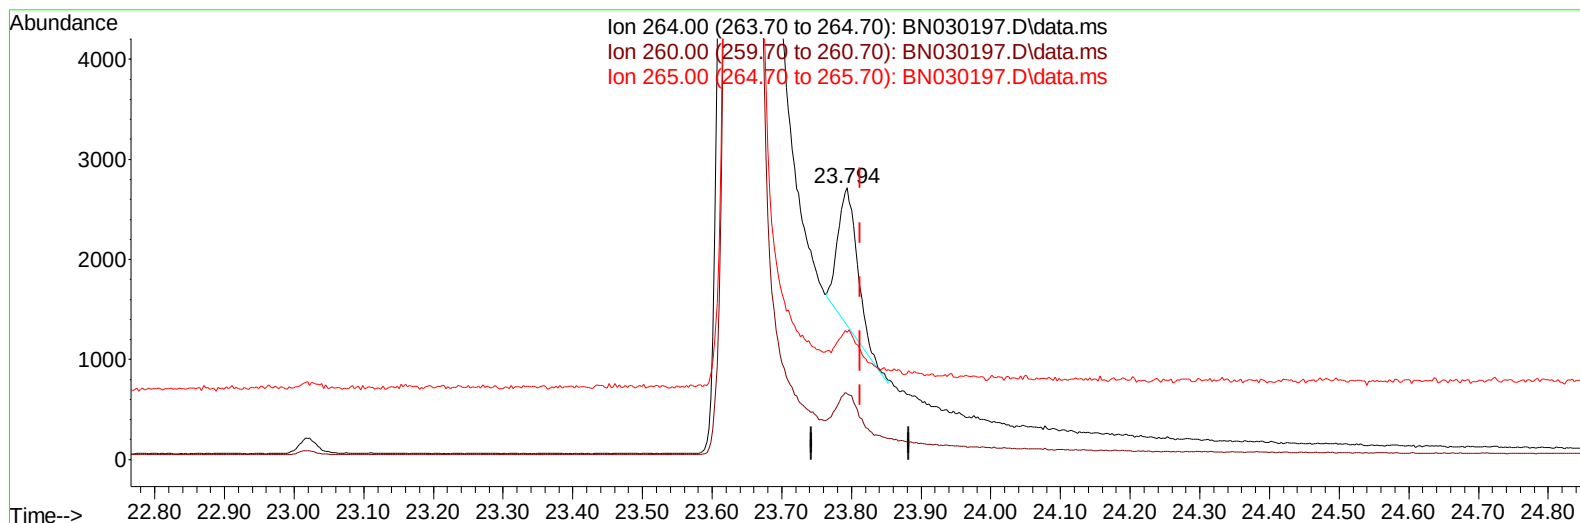

TIC: BN030197.D\data.ms

(23) Perylene-d12 (I)

23.794min (-0.018) 0.40 ng/ul m

response 2607

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	29.20	24.24
265.00	110.00	46.76#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
 Data File : BN030197.D
 Acq On : 03 Mar 2024 01:20
 Operator : MA/JU
 Sample : P1501-11
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E10B2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/04/2024
 Supervised By :mohammad ahmed 03/05/2024

Quant Time: Mar 03 22:49:54 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 02 16:09:30 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.834	152		1496	0.400	ng/ul	0.00
4) Naphthalene-d8	10.623	136		3872	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.479	164		1947	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.234	188		3845	0.400	ng/ul	#-0.01
17) Chrysene-d12	21.453	240		2846	0.400	ng/ul	0.00
23) Perylene-d12	23.794	264		2607m	0.400	ng/ul	-0.02
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.302	96		7765	3.749	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.234	152		1710	0.342	ng/ul	0.00
18) Fluoranthene-d10	19.272	212		3581	0.386	ng/ul	-0.01
Target Compounds							
							Qvalue
5) Naphthalene	10.672	128		252	0.022	ng/ul#	49

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
Data File : BN030197.D
Acq On : 03 Mar 2024 01:20
Operator : MA/JU
Sample : P1501-11
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E10B2

Manual IntegrationsAPPROVED

Quant Time: Mar 03 22:49:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 02 16:09:30 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/04/2024
Supervised By :mohammad ahmed 03/05/2024

