




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
Data File : BN030224.D
Acq On : 03 Mar 2024 18:47
Operator : MA/JU
Sample : PB159151BL
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK151

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/04/2024
Supervised By :mohammad ahmed 03/05/2024

Quant Time: Mar 03 22:54:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 02 16:09:30 2024
Response via : Initial Calibration

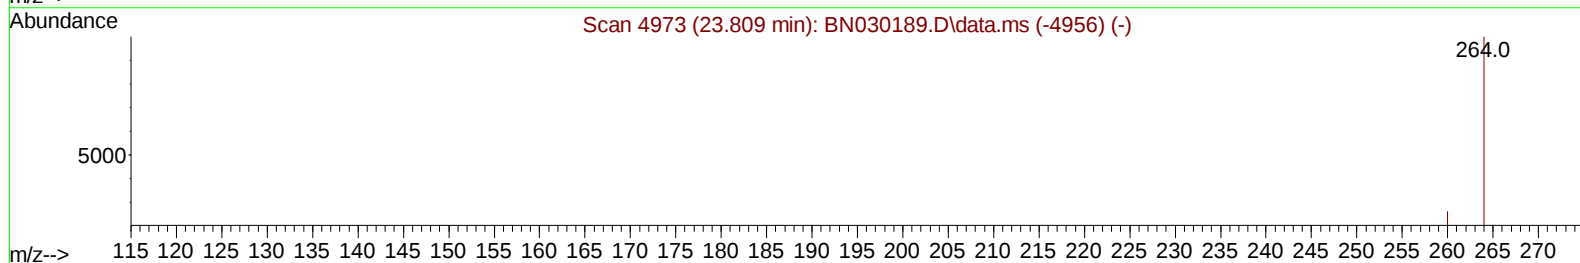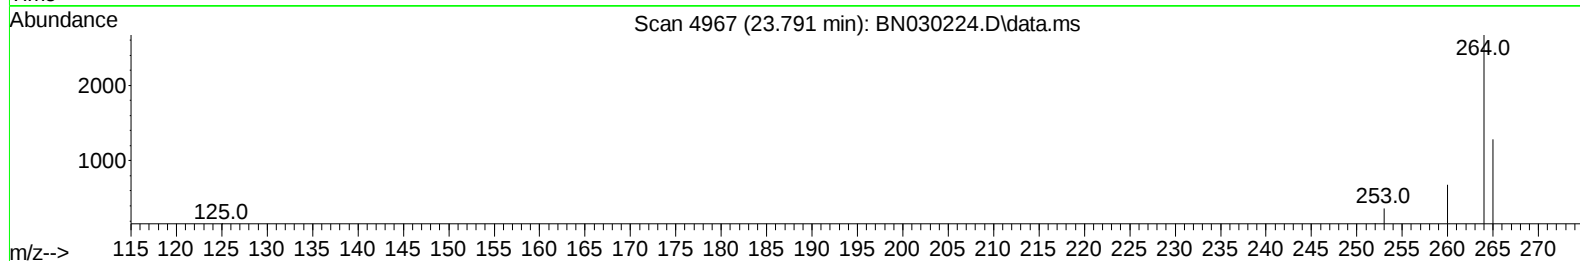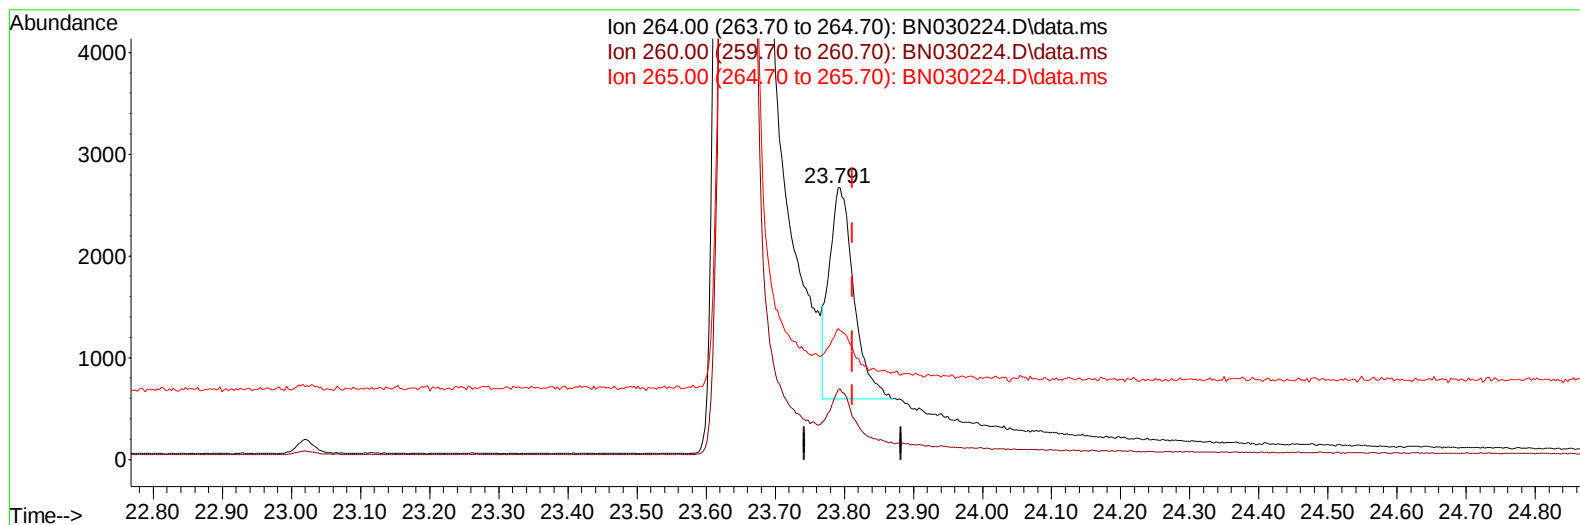

TIC: BN030224.D\data.ms

(23) Perylene-d12 (I)

23.791min (-0.021) 0.40 ng/u1

response 5154

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	29.20	25.55
265.00	110.00	48.26#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
Data File : BN030224.D
Acq On : 03 Mar 2024 18:47
Operator : MA/JU
Sample : PB159151BL
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK151

Manual IntegrationsAPPROVED

Quant Time: Mar 03 22:54:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 02 16:09:30 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/04/2024
Supervised By :mohammad ahmed 03/05/2024

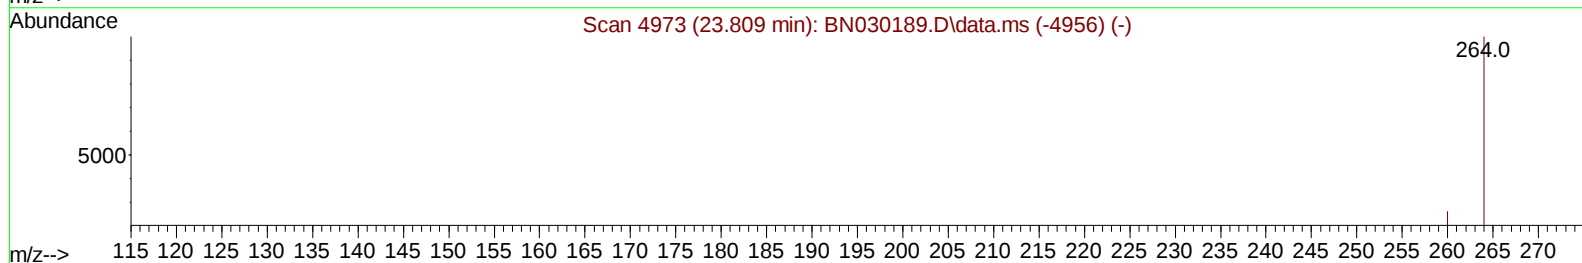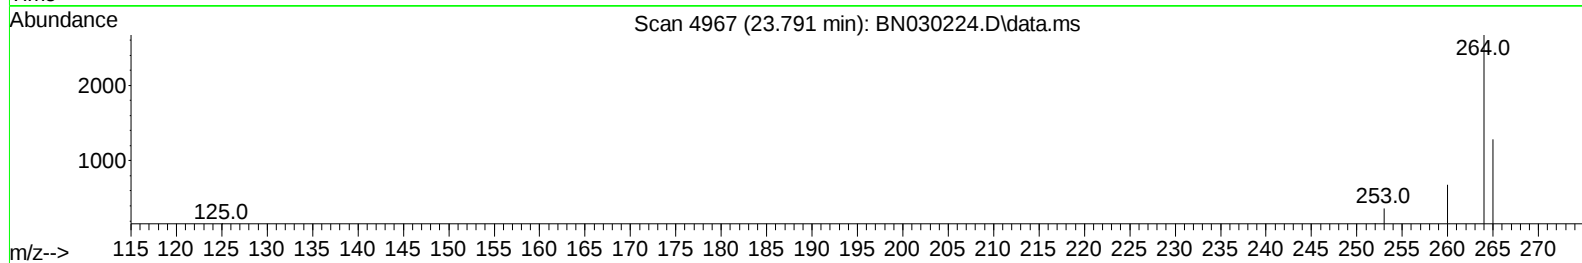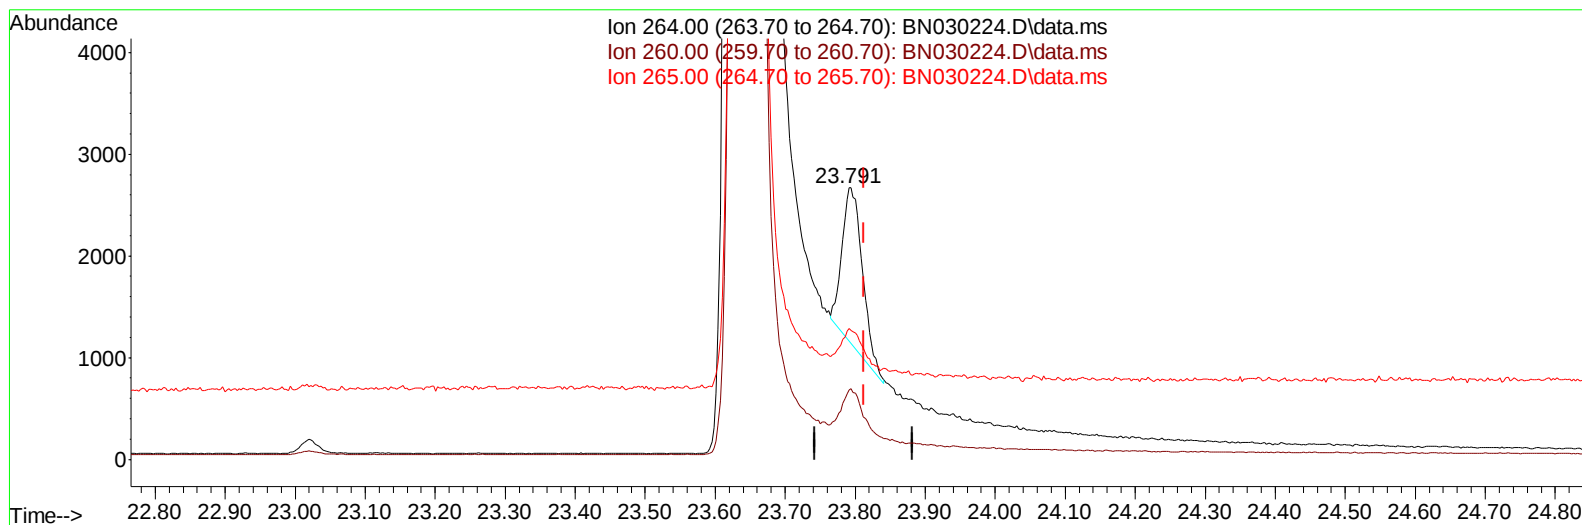

TIC: BN030224.D\data.ms

(23) Perylene-d12 (I)

23.791min (-0.021) 0.40 ng/ul m

response 3033

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	29.20	25.55
265.00	110.00	48.26#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
 Data File : BN030224.D
 Acq On : 03 Mar 2024 18:47
 Operator : MA/JU
 Sample : PB159151BL
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK151

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/04/2024
 Supervised By :mohammad ahmed 03/05/2024

Quant Time: Mar 03 22:54:27 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 02 16:09:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.830	152	1352	0.400	ng/ul	0.00
4) Naphthalene-d8	10.623	136	3554	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.474	164	1762	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.230	188	3483	0.400	ng/ul	#-0.02
17) Chrysene-d12	21.453	240	2785	0.400	ng/ul	0.00
23) Perylene-d12	23.791	264	3033m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.302	96	10660	5.695	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.229	152	1443	0.314	ng/ul	-0.01
18) Fluoranthene-d10	19.272	212	2739	0.302	ng/ul	-0.01

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
Data File : BN030224.D
Acq On : 03 Mar 2024 18:47
Operator : MA/JU
Sample : PB159151BL
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK151

Manual IntegrationsAPPROVED

Quant Time: Mar 03 22:54:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 02 16:09:30 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/04/2024
Supervised By :mohammad ahmed 03/05/2024

