




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
Data File : BN030225.D
Acq On : 03 Mar 2024 19:23
Operator : MA/JU
Sample : PB159243BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK243

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/04/2024
Supervised By :mohammad ahmed 03/05/2024

Quant Time: Mar 03 22:54:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 02 16:09:30 2024
Response via : Initial Calibration

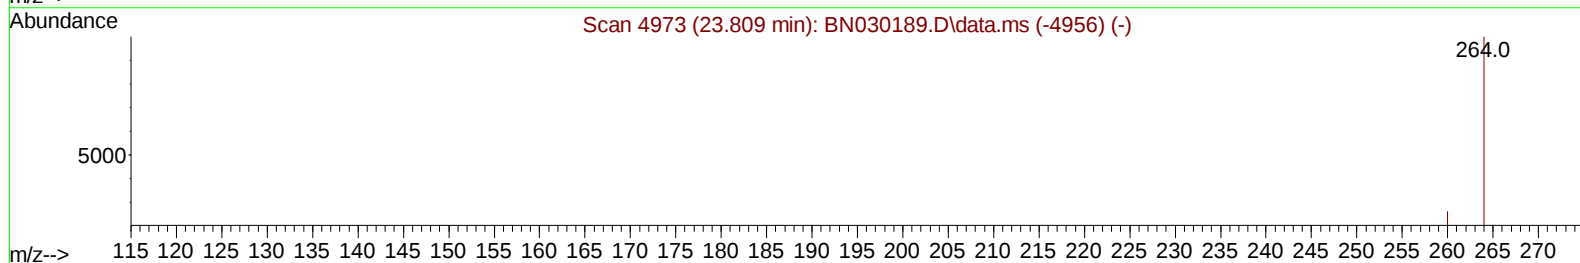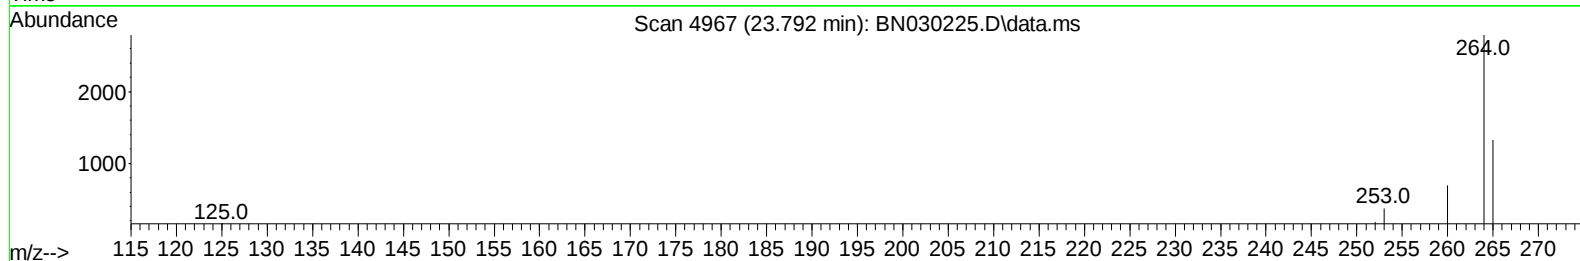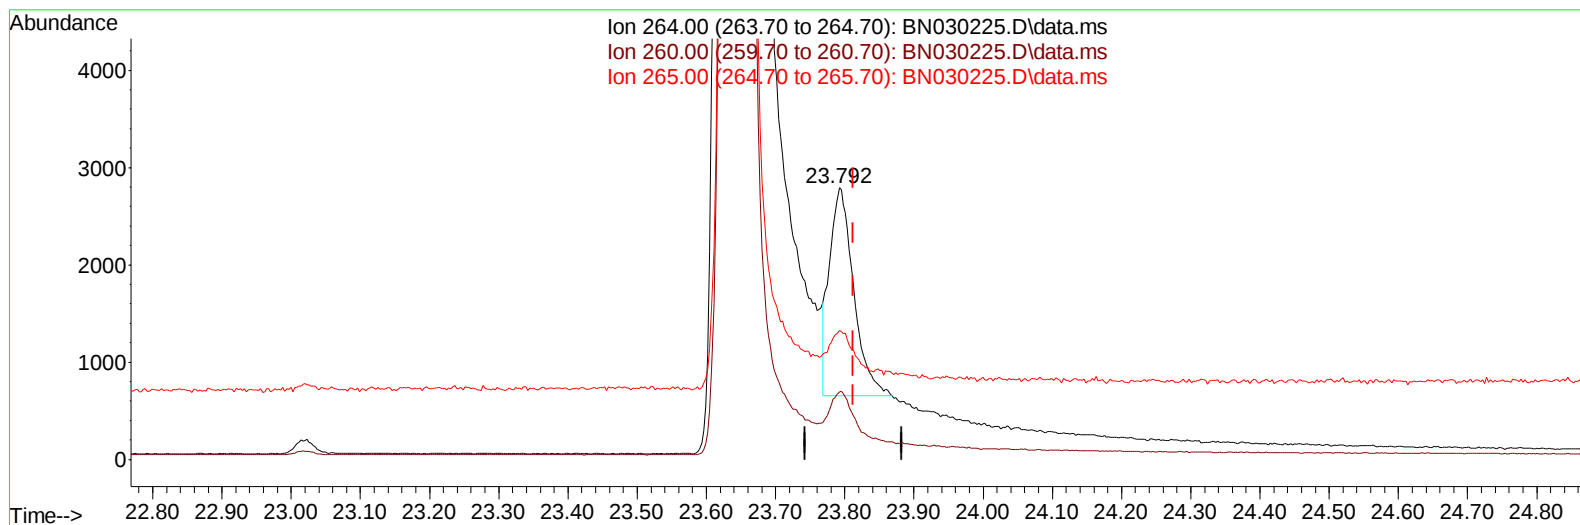

TIC: BN030225.D\data.ms

(23) Perylene-d12 (I)

23.792min (-0.020) 0.40 ng/u1

response 5159

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	29.20	24.90
265.00	110.00	47.47#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
Data File : BN030225.D
Acq On : 03 Mar 2024 19:23
Operator : MA/JU
Sample : PB159243BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK243

Manual IntegrationsAPPROVED

Quant Time: Mar 03 22:54:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 02 16:09:30 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/04/2024
Supervised By :mohammad ahmed 03/05/2024

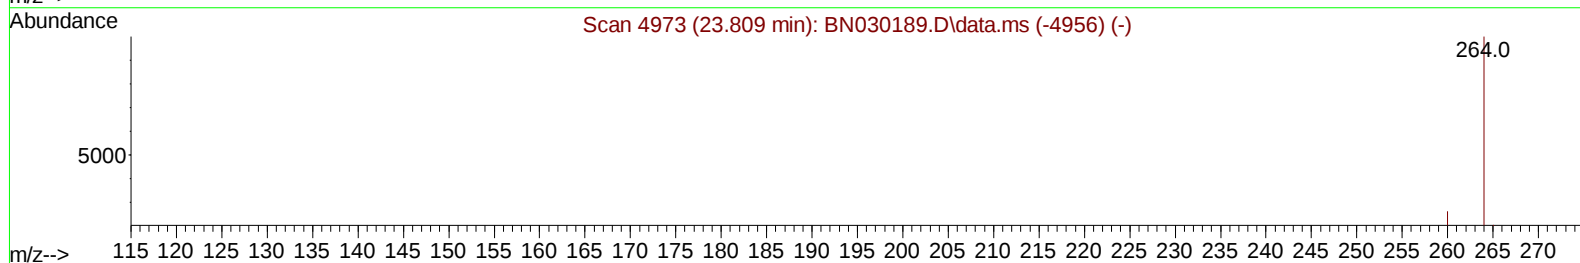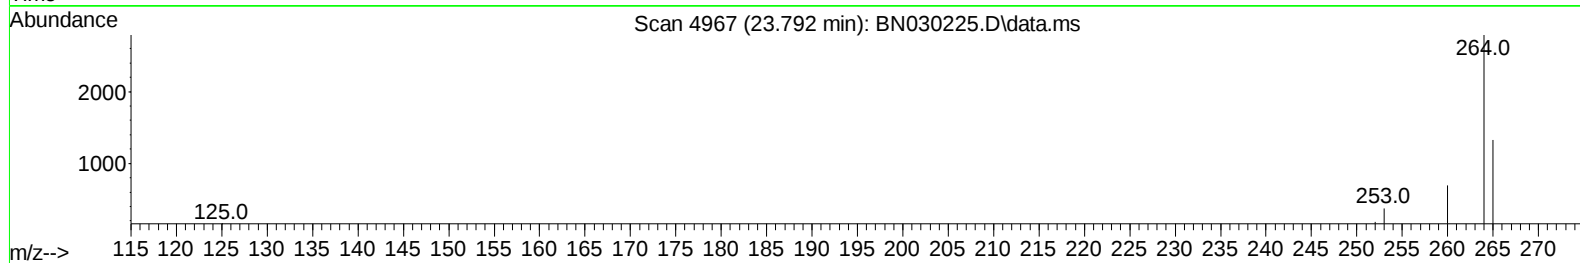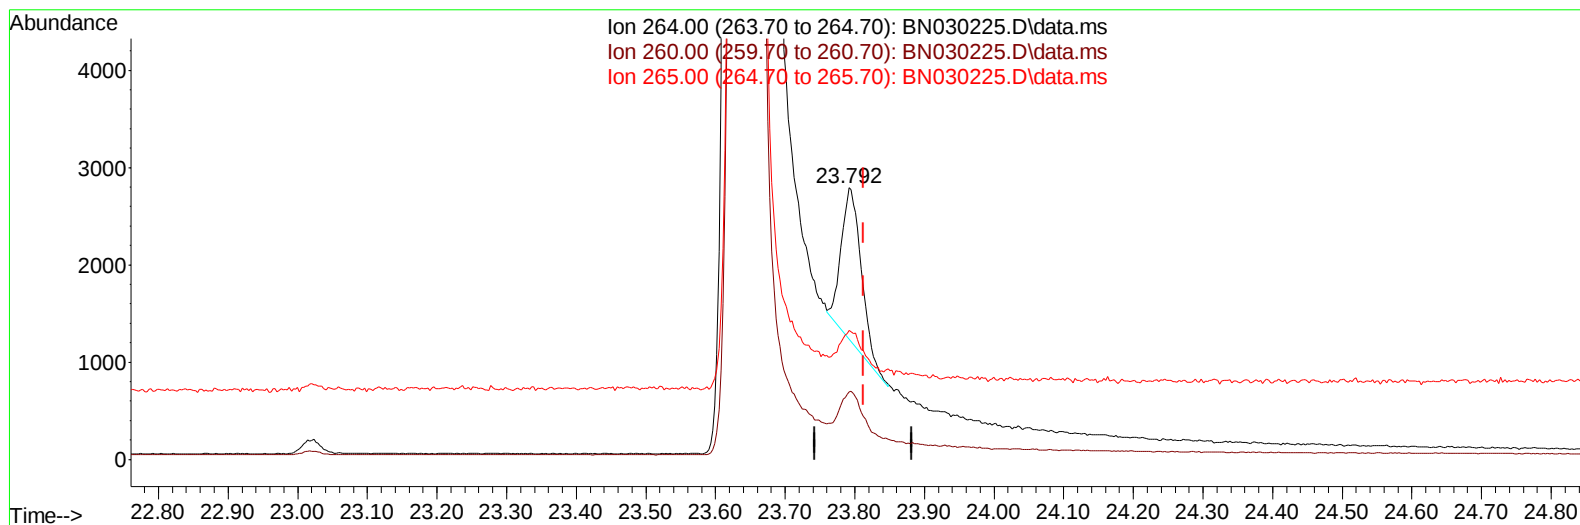

TIC: BN030225.D\data.ms

(23) Perylene-d12 (I)

23.792min (-0.020) 0.40 ng/ul m

response 3081

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	29.20	24.90
265.00	110.00	47.47#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
 Data File : BN030225.D
 Acq On : 03 Mar 2024 19:23
 Operator : MA/JU
 Sample : PB159243BL
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK243

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/04/2024
 Supervised By :mohammad ahmed 03/05/2024

Quant Time: Mar 03 22:54:34 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 02 16:09:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.829	152	1510	0.400	ng/ul	0.00
4) Naphthalene-d8	10.623	136	4005	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.475	164	1989	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.231	188	3850	0.400	ng/ul	#-0.02
17) Chrysene-d12	21.451	240	2945	0.400	ng/ul	# 0.00
23) Perylene-d12	23.792	264	3081m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.302	96	12928	6.184	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.228	152	1708	0.330	ng/ul	-0.01
18) Fluoranthene-d10	19.268	212	3178	0.331	ng/ul	-0.01

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
Data File : BN030225.D
Acq On : 03 Mar 2024 19:23
Operator : MA/JU
Sample : PB159243BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK243

Manual IntegrationsAPPROVED

Quant Time: Mar 03 22:54:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 02 16:09:30 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/04/2024
Supervised By :mohammad ahmed 03/05/2024

