




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
Data File : BN030252.D
Acq On : 04 Mar 2024 12:12
Operator : MA/JU
Sample : P1501-19
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E10B8

Manual IntegrationsAPPROVED

Quant Time: Mar 04 13:18:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 04 05:54:20 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/04/2024
Supervised By :mohammad ahmed 03/05/2024

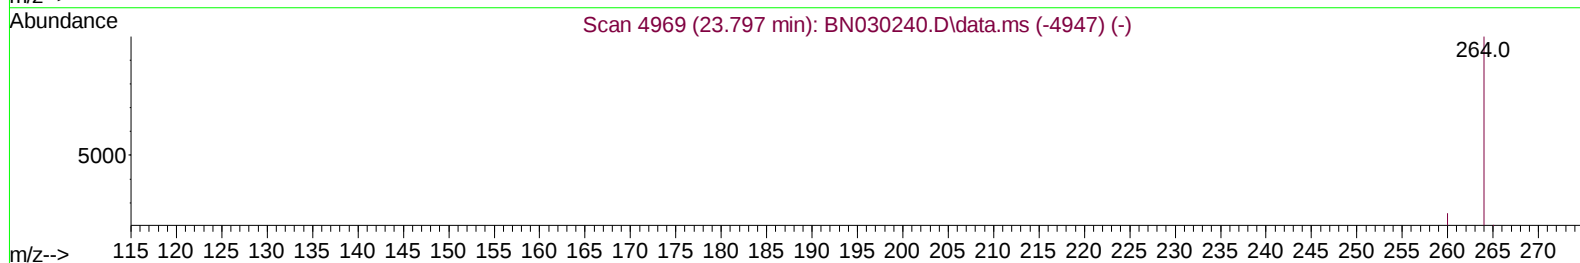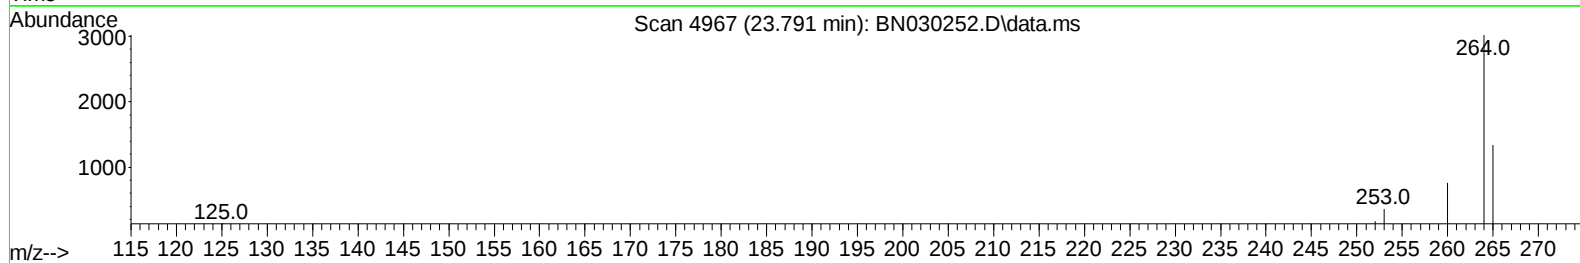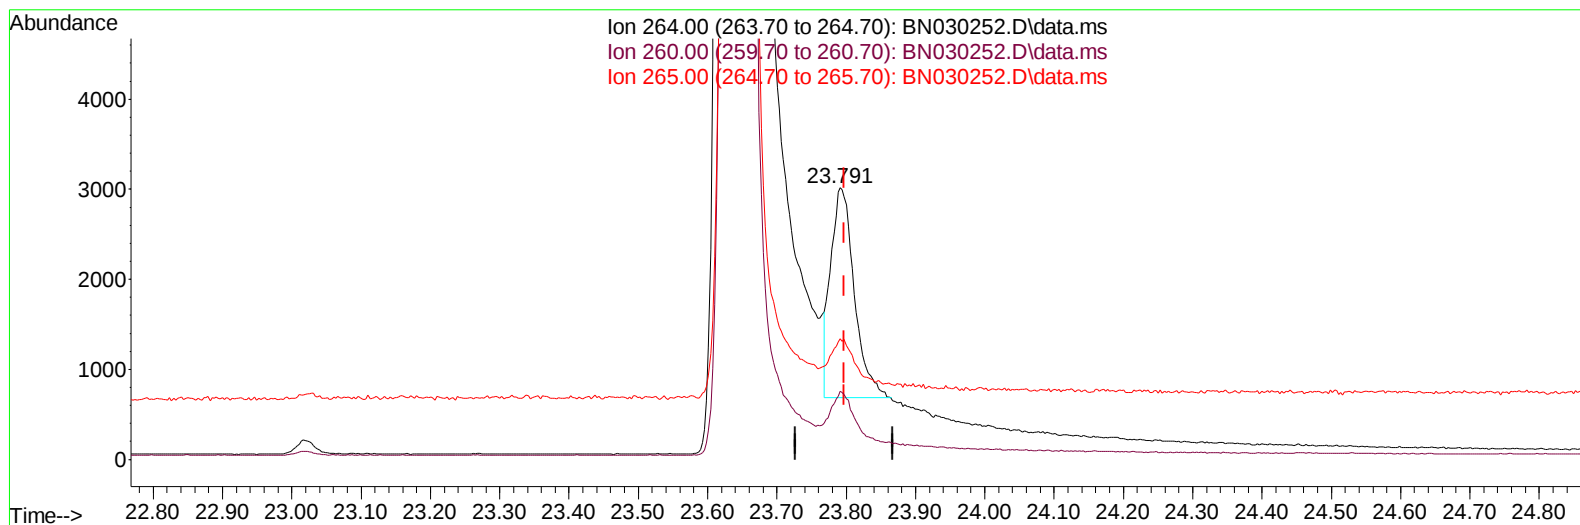

TIC: BN030252.D\data.ms

(23) Perylene-d12 (I)

23.791min (-0.006) 0.40 ng/u1

response 5507

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	29.20	25.11
265.00	110.00	44.44#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
 Data File : BN030252.D
 Acq On : 04 Mar 2024 12:12
 Operator : MA/JU
 Sample : P1501-19
 Misc :
 ALS Vial : 75 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E10B8

Manual IntegrationsAPPROVED

Quant Time: Mar 04 13:18:20 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 04 05:54:20 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/04/2024
 Supervised By :mohammad ahmed 03/05/2024

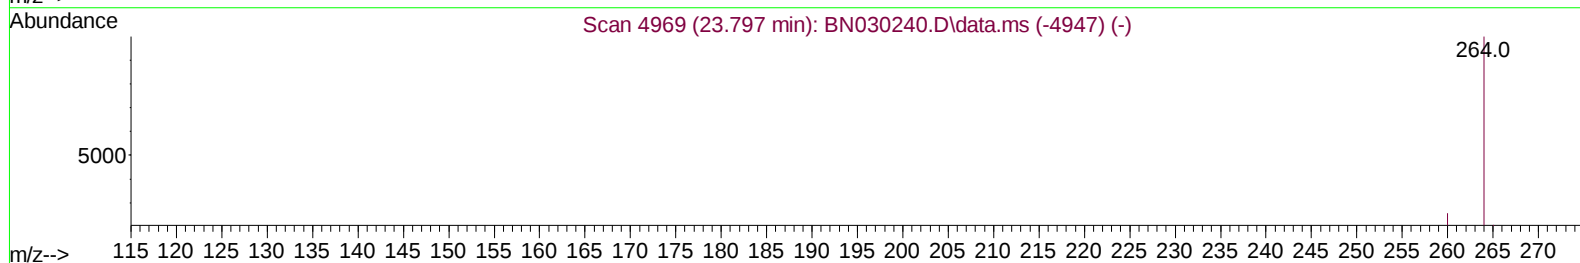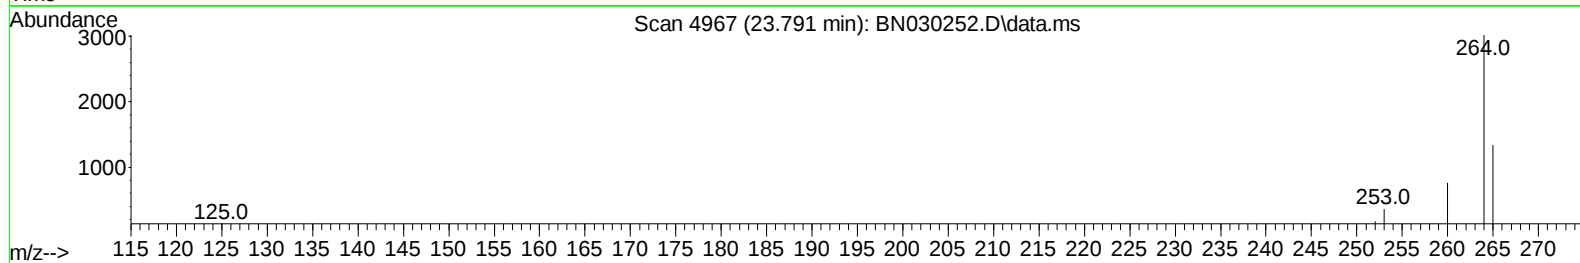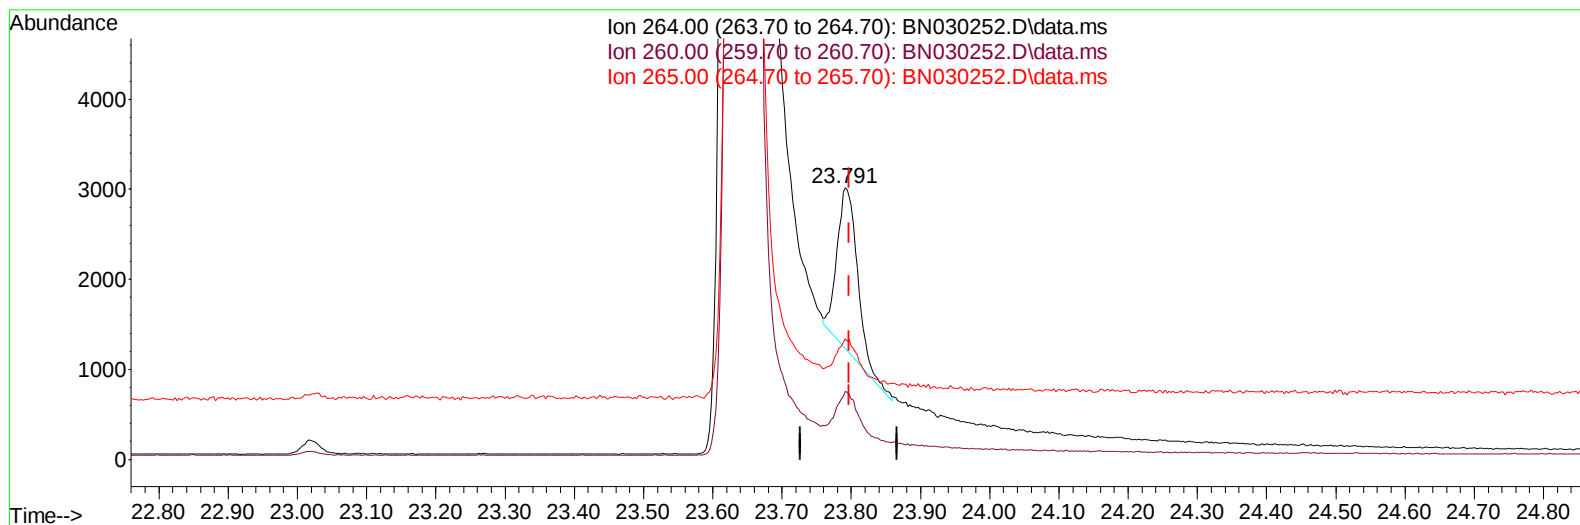

TIC: BN030252.D\data.ms

(23) Perylene-d12 (I)

23.791min (-0.006) 0.40 ng/ul m

response 3652

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	29.20	25.11
265.00	110.00	44.44#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
 Data File : BN030252.D
 Acq On : 04 Mar 2024 12:12
 Operator : MA/JU
 Sample : P1501-19
 Misc :
 ALS Vial : 75 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E10B8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/04/2024
 Supervised By :mohammad ahmed 03/05/2024

Quant Time: Mar 04 13:18:20 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 04 05:54:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.830	152	1382	0.400	ng/ul	0.00
4) Naphthalene-d8	10.623	136	3598	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.474	164	1820	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.230	188	3751	0.400	ng/ul #	0.00
17) Chrysene-d12	21.453	240	3234	0.400	ng/ul #	0.00
23) Perylene-d12	23.791	264	3652m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.302	96	6466	3.380	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.229	152	1253	0.269	ng/ul	0.00
18) Fluoranthene-d10	19.267	212	3202	0.304	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
Data File : BN030252.D
Acq On : 04 Mar 2024 12:12
Operator : MA/JU
Sample : P1501-19
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E10B8

Manual IntegrationsAPPROVED

Quant Time: Mar 04 13:18:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 04 05:54:20 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/04/2024
Supervised By :mohammad ahmed 03/05/2024

