




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
Data File : BN030253.D
Acq On : 04 Mar 2024 12:48
Operator : MA/JU
Sample : P1501-20
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E10B9

Manual IntegrationsAPPROVED

Quant Time: Mar 04 13:20:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 04 05:54:20 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/04/2024
Supervised By :mohammad ahmed 03/05/2024

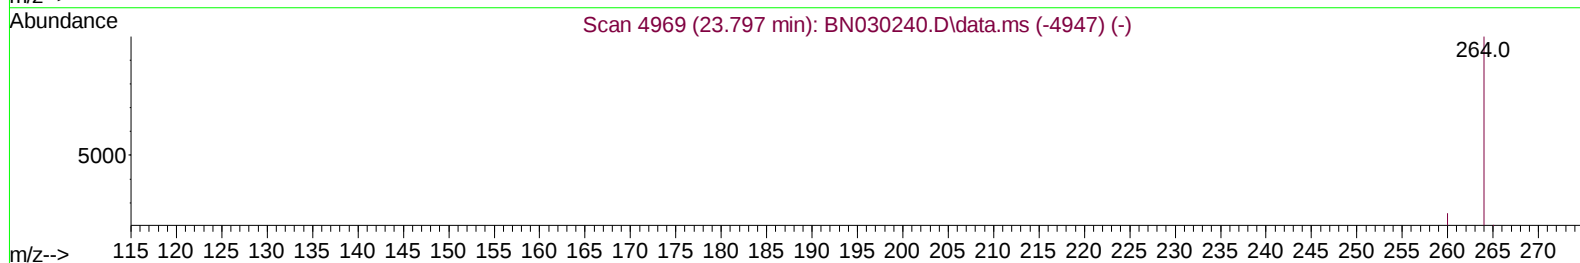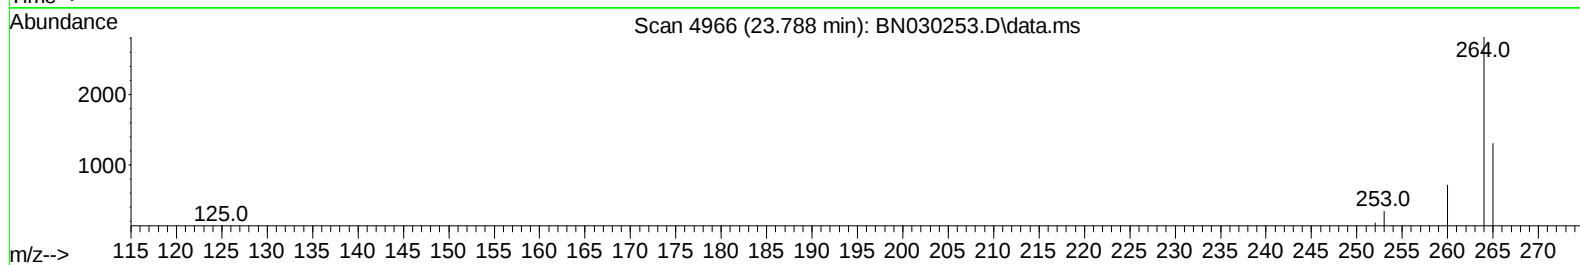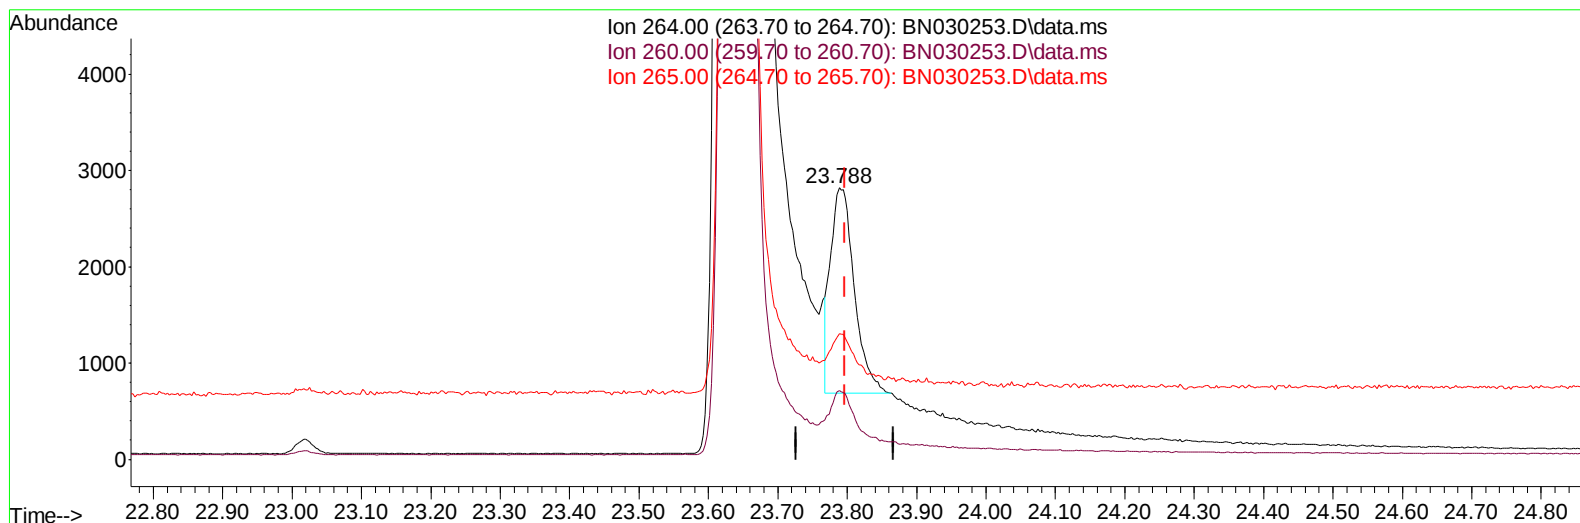

TIC: BN030253.D\data.ms

(23) Perylene-d12 (I)

23.788min (-0.009) 0.40 ng/u1

response 5061

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	29.20	25.26
265.00	110.00	46.36#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
 Data File : BN030253.D
 Acq On : 04 Mar 2024 12:48
 Operator : MA/JU
 Sample : P1501-20
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E10B9

Manual IntegrationsAPPROVED

Quant Time: Mar 04 13:20:59 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 04 05:54:20 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/04/2024
 Supervised By :mohammad ahmed 03/05/2024

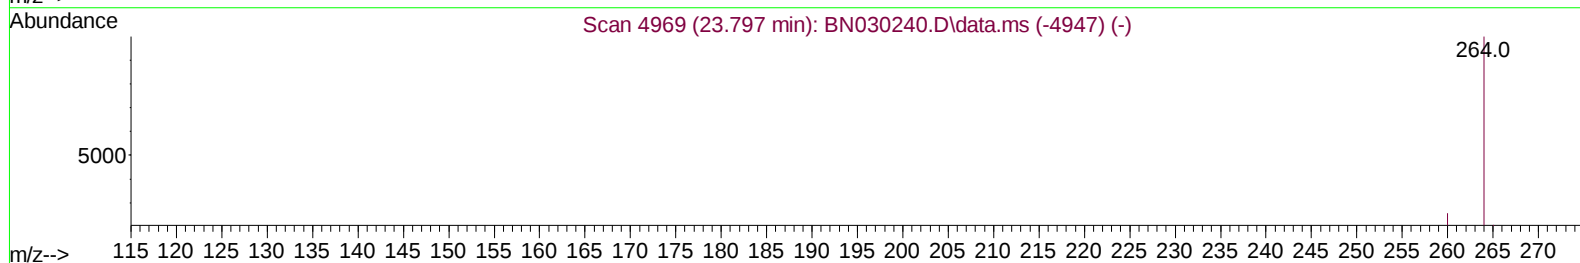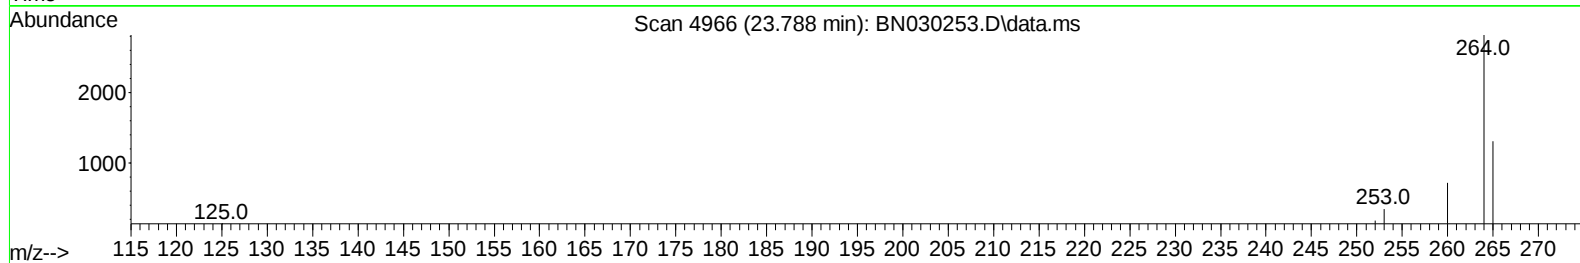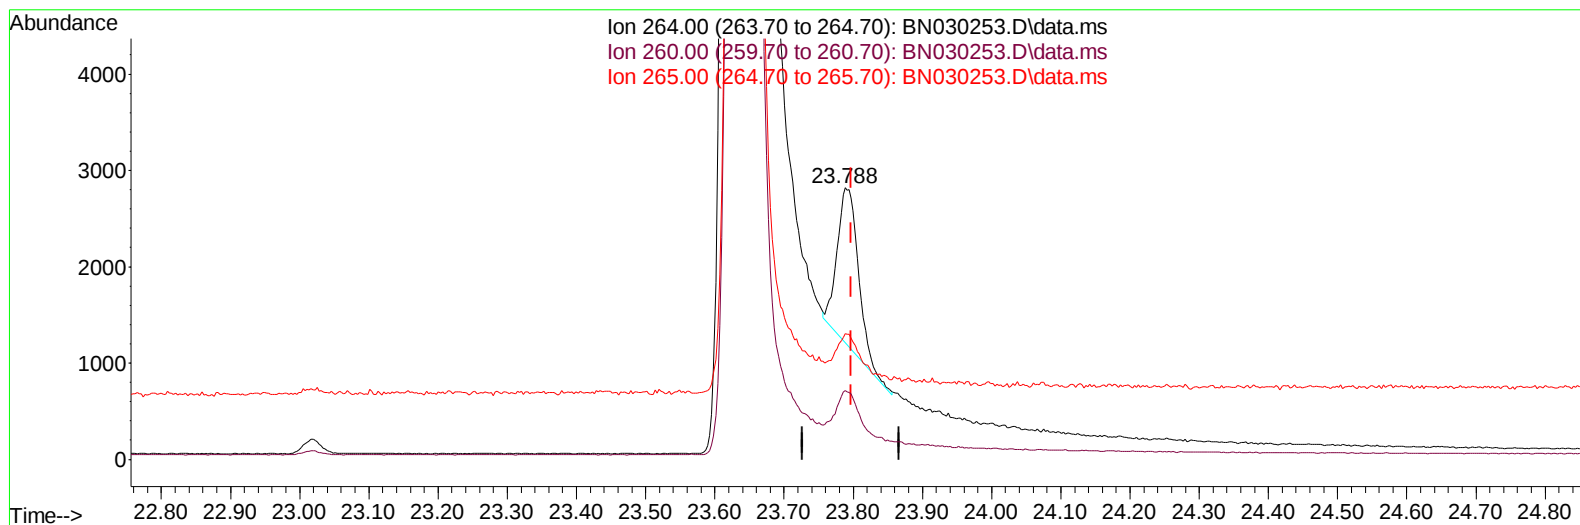

TIC: BN030253.D\data.ms

(23) Perylene-d12 (I)

23.788min (-0.009) 0.40 ng/ul m

response 3425

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	29.20	25.26
265.00	110.00	46.36#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
 Data File : BN030253.D
 Acq On : 04 Mar 2024 12:48
 Operator : MA/JU
 Sample : P1501-20
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E10B9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/04/2024
 Supervised By :mohammad ahmed 03/05/2024

Quant Time: Mar 04 13:20:59 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 04 05:54:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.830	152	1523	0.400	ng/ul	0.00
4) Naphthalene-d8	10.617	136	3962	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.474	164	1989	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.230	188	3910	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.450	240	3152	0.400	ng/ul	# 0.00
23) Perylene-d12	23.788	264	3425m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.302	96	6894	3.270	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.229	152	1527	0.298	ng/ul	0.00
18) Fluoranthene-d10	19.267	212	3216	0.313	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
Data File : BN030253.D
Acq On : 04 Mar 2024 12:48
Operator : MA/JU
Sample : P1501-20
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E10B9

Manual IntegrationsAPPROVED

Quant Time: Mar 04 13:20:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 04 05:54:20 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/04/2024
Supervised By :mohammad ahmed 03/05/2024

