

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
 Data File : BN030188.D
 Acq On : 02 Mar 2024 19:19
 Operator : MA/JU
 Sample : P1501-18
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E10B6

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 03/04/2024
 Supervised By :mohammad ahmed 03/05/2024

Quant Time: Mar 03 22:48:39 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 02 16:09:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.834	152	1279	0.400	ng/ul	0.00
4) Naphthalene-d8	10.627	136	3416	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.477	164	1713	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.233	188	3251	0.400	ng/ul	#-0.01
17) Chrysene-d12	21.456	240	2196	0.400	ng/ul	0.00
23) Perylene-d12	23.794	264	2039m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.302	96	8607	4.861	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.233	152	1925	0.436	ng/ul	0.00
18) Fluoranthene-d10	19.271	212	3833	0.536	ng/ul	-0.01
Target Compounds						Qvalue
5) Naphthalene	10.676	128	359	0.036	ng/ul#	65

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
Data File : BN030188.D
Acq On : 02 Mar 2024 19:19
Operator : MA/JU
Sample : P1501-18
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
E10B6

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 03/04/2024
Supervised By :mohammad ahmed 03/05/2024

Quant Time: Mar 03 22:48:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 02 16:09:30 2024
Response via : Initial Calibration

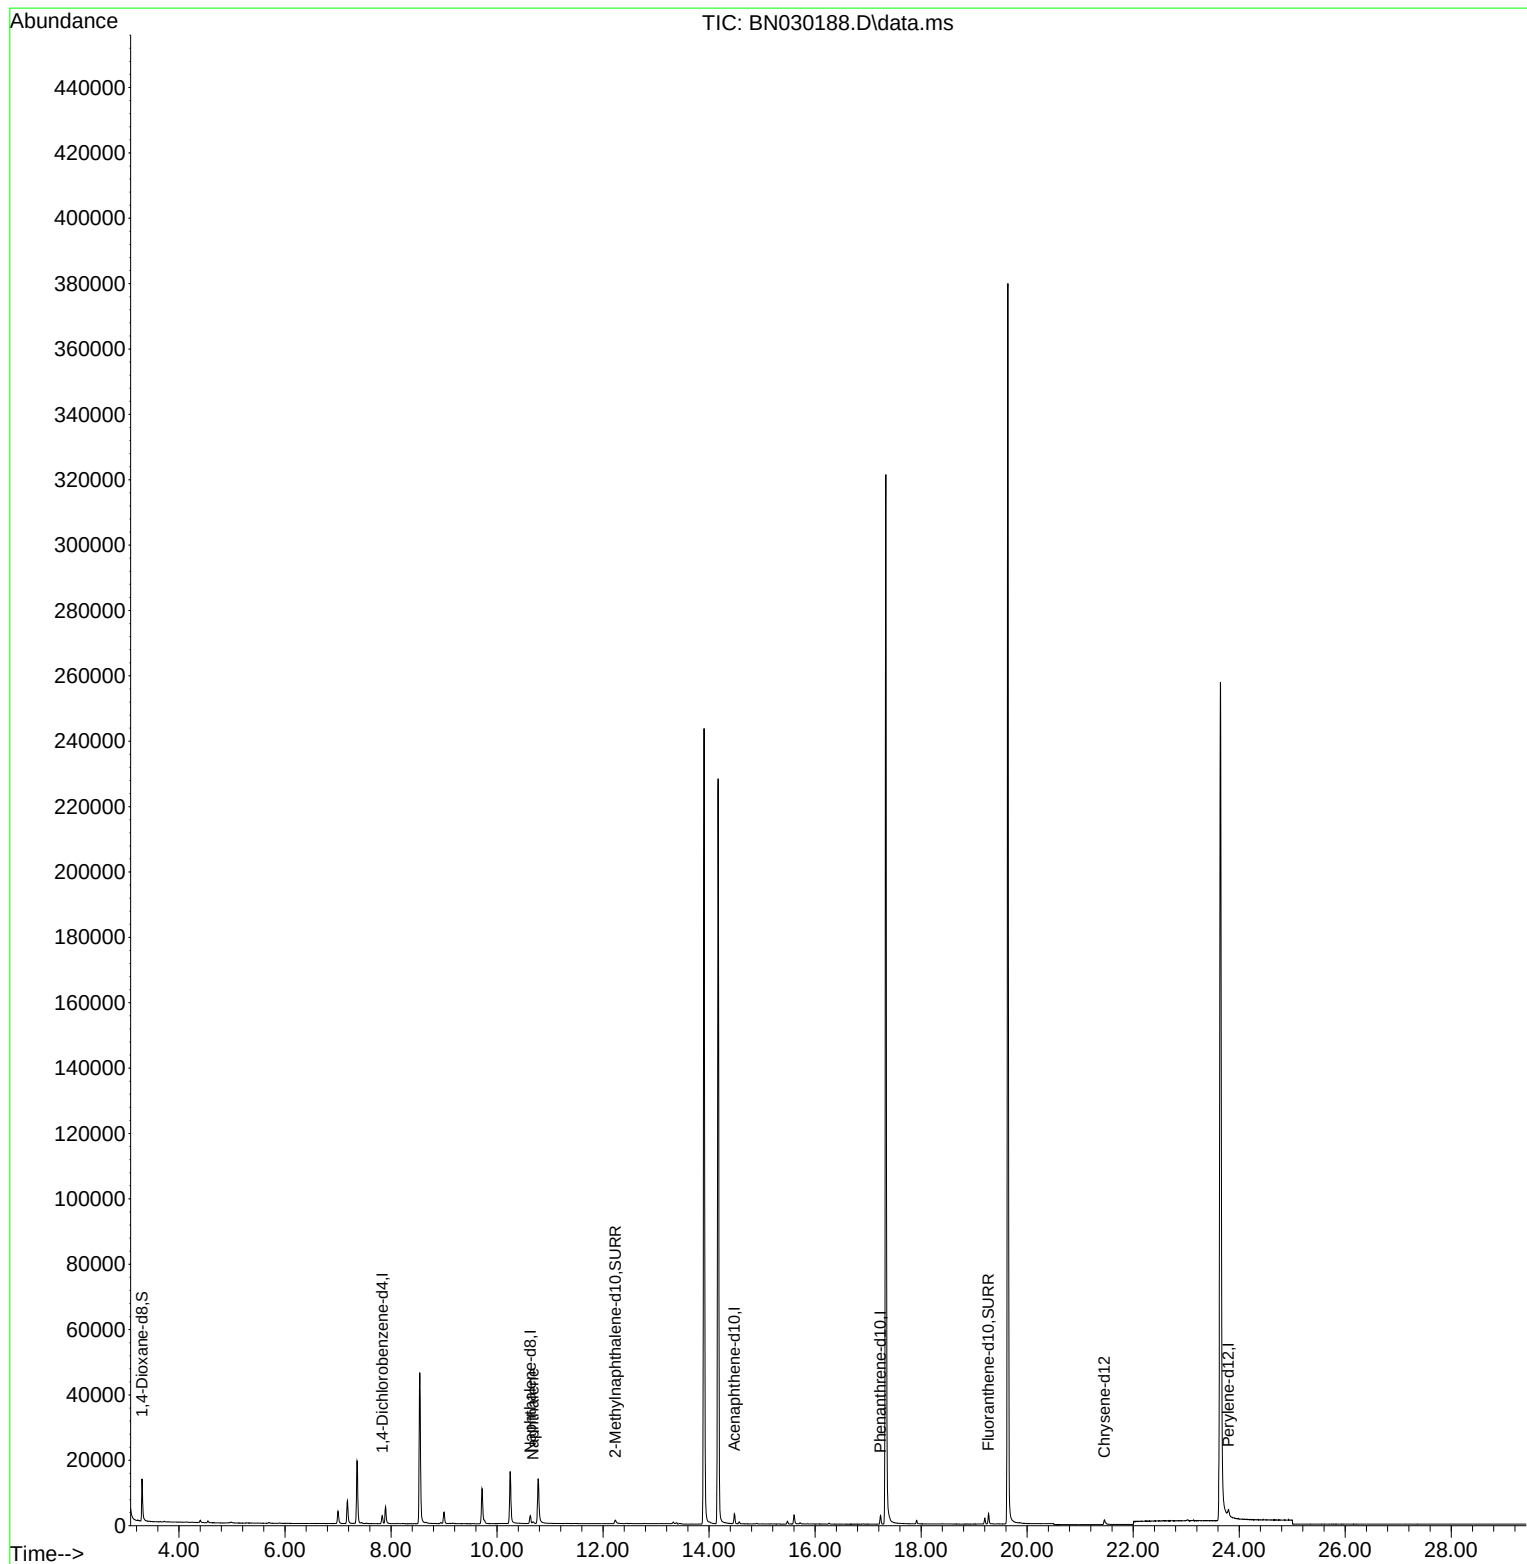

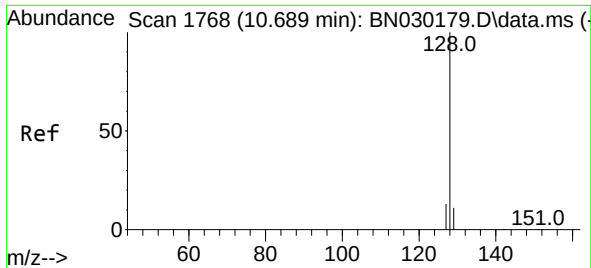

#5

Naphthalene

Concen: 0.036 ng/ul

RT: 10.676 min Scan# 1

Delta R.T. -0.012 min

Lab File: BN030188.D


Acq: 02 Mar 2024 19:19

Instrument :

BNA_N

ClientSampleId :

E10B6

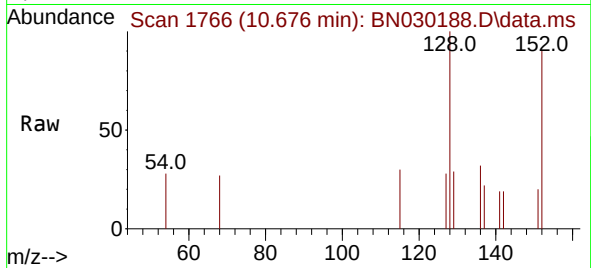

Tgt Ion:128 Resp: 359

Ion Ratio Lower Upper

128 100

129 29.2 11.0 16.4

127 28.5 12.3 18.5

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 03/04/2024

Supervised By :mohammad ahmed 03/05/2024

