

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
 Data File : BN030196.D
 Acq On : 03 Mar 2024 00:44
 Operator : MA/JU
 Sample : P1501-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E10B1

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 03/04/2024
 Supervised By :mohammad ahmed 03/05/2024

Quant Time: Mar 03 22:49:47 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 02 16:09:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.834	152	1324	0.400	ng/ul	0.00
4) Naphthalene-d8	10.628	136	3373	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.479	164	1786	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.234	188	3627	0.400	ng/ul	#-0.01
17) Chrysene-d12	21.453	240	2827	0.400	ng/ul	0.00
23) Perylene-d12	23.794	264	2730m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.302	96	6681	3.645	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.228	152	1682	0.386	ng/ul	-0.01
18) Fluoranthene-d10	19.272	212	3824	0.415	ng/ul	-0.01
Target Compounds						Qvalue
5) Naphthalene	10.672	128	243	0.024	ng/ul#	50

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
Data File : BN030196.D
Acq On : 03 Mar 2024 00:44
Operator : MA/JU
Sample : P1501-10
Misc :
ALS Vial : 16 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
E10B1

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 03/04/2024
Supervised By :mohammad ahmed 03/05/2024


Quant Time: Mar 03 22:49:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 02 16:09:30 2024
Response via : Initial Calibration

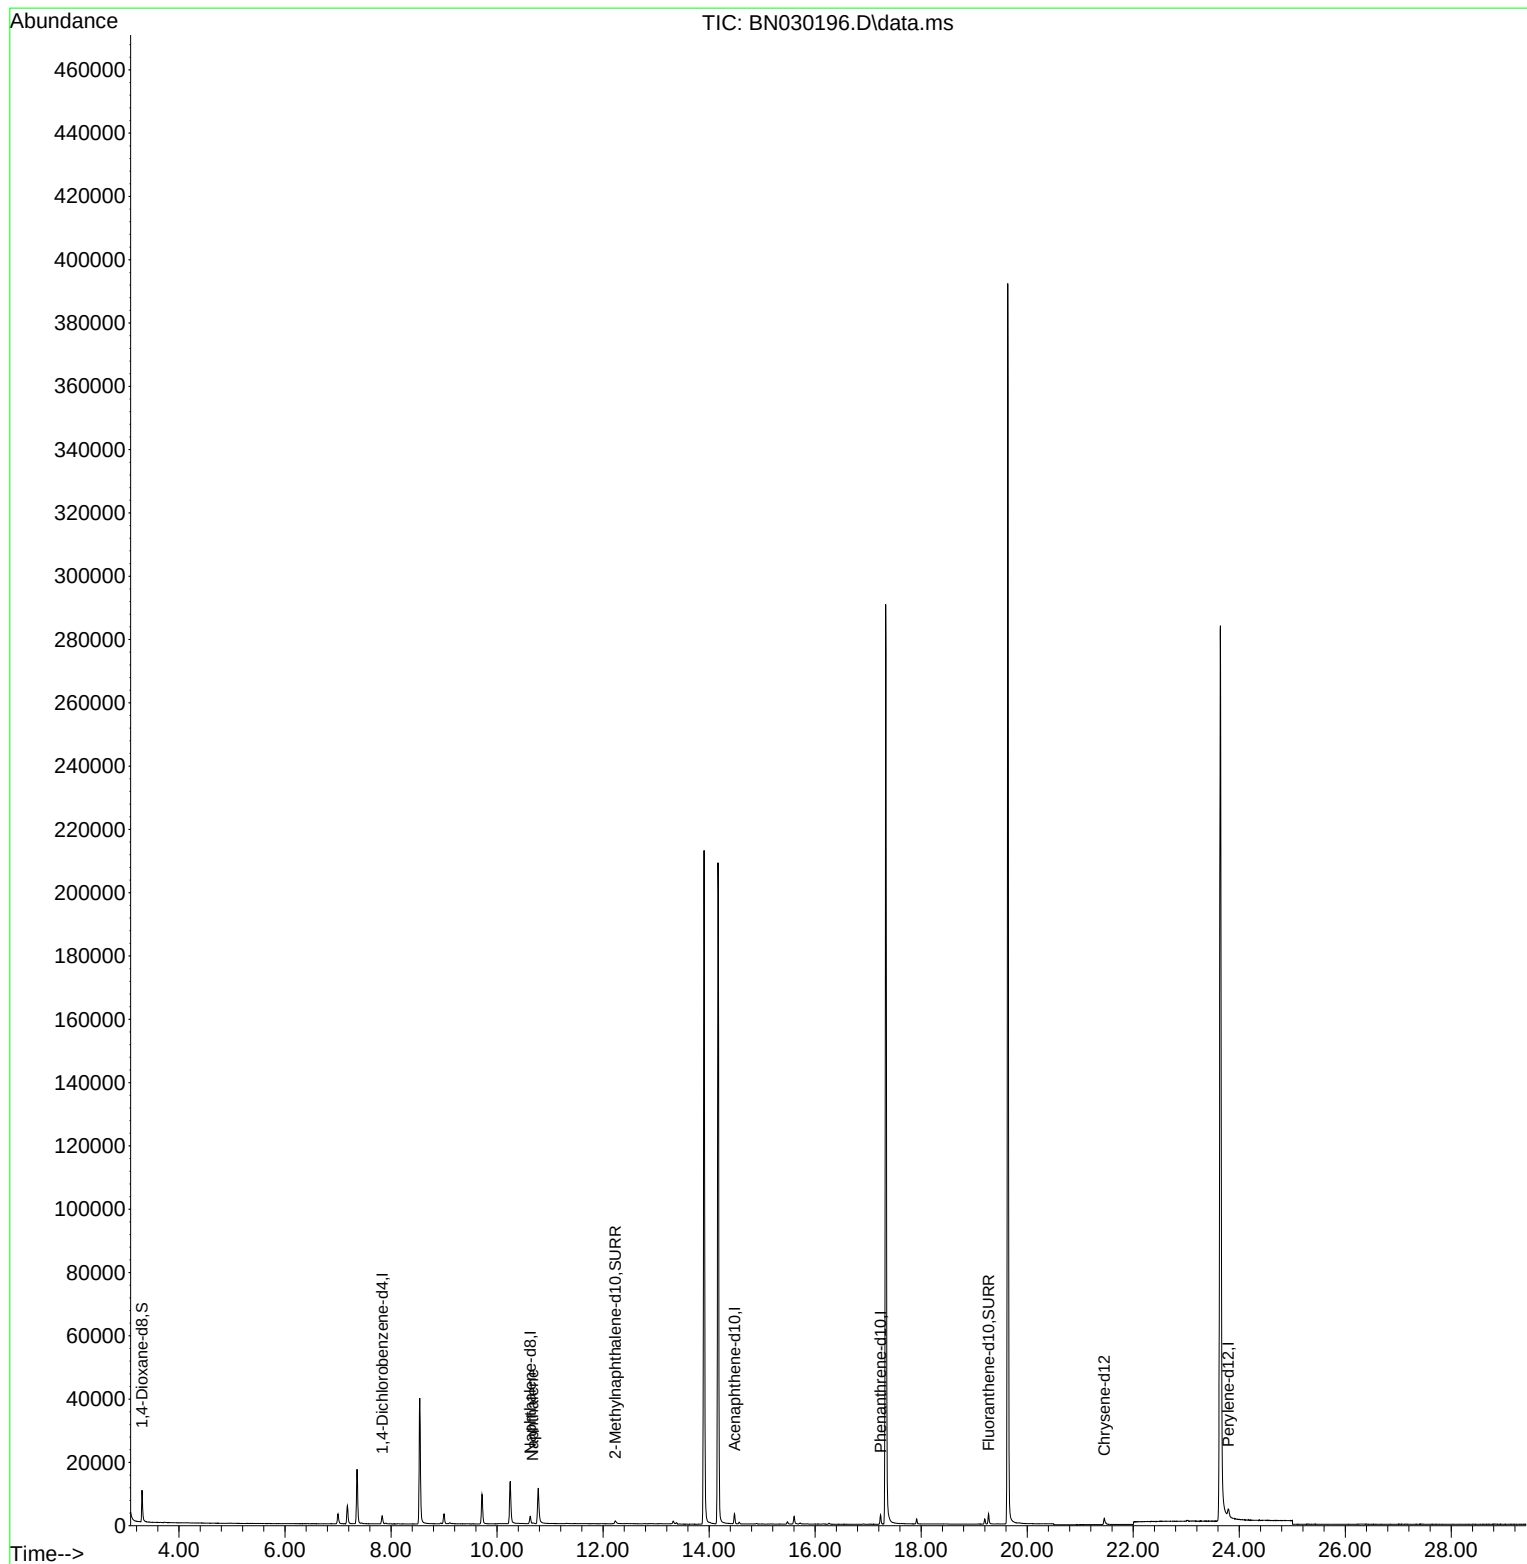

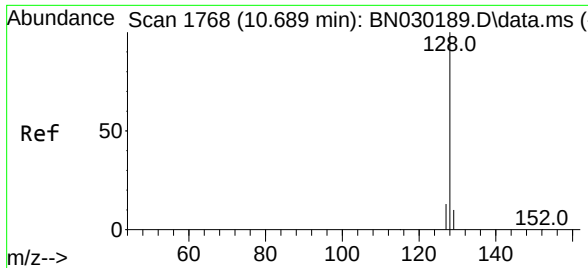

#5
Naphthalene
Concen: 0.024 ng/ul
RT: 10.672 min Scan# 11
Delta R.T. -0.016 min
Lab File: BN030196.D
Acq: 03 Mar 2024 00:44

Instrument :
BNA_N
ClientSampleId :
E10B1

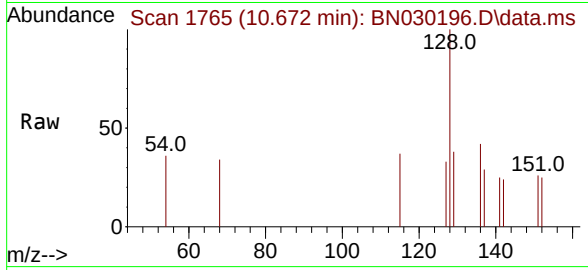

Tgt Ion:	128	Resp:	24
Ion	Ratio	Lower	Upper
128	100		
129	37.6	11.0	16.4
127	33.0	12.3	18.5

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 03/04/2024
Supervised By :mohammad ahmed 03/05/2024

