

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
 Data File : BN030199.D
 Acq On : 03 Mar 2024 02:32
 Operator : MA/JU
 Sample : P1501-13
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E10B4

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 03/04/2024
 Supervised By :mohammad ahmed 03/05/2024

Quant Time: Mar 03 22:50:09 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 02 16:09:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.834	152	1535	0.400	ng/u1	0.00
4) Naphthalene-d8	10.623	136	4079	0.400	ng/u1	#-0.02
9) Acenaphthene-d10	14.479	164	2082	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.235	188	4166	0.400	ng/u1	#-0.01
17) Chrysene-d12	21.453	240	3214	0.400	ng/u1	# 0.00
23) Perylene-d12	23.794	264	2950m	0.400	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.302	96	7459	3.510	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.229	152	1635	0.310	ng/u1	-0.01
18) Fluoranthene-d10	19.272	212	3898	0.372	ng/u1	0.00
Target Compounds						
5) Naphthalene	10.672	128	256	0.021	ng/u1#	Qvalue 49

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
Data File : BN030199.D
Acq On : 03 Mar 2024 02:32
Operator : MA/JU
Sample : P1501-13
Misc :
ALS Vial : 19 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
E10B4

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 03/04/2024
Supervised By :mohammad ahmed 03/05/2024


Quant Time: Mar 03 22:50:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 02 16:09:30 2024
Response via : Initial Calibration

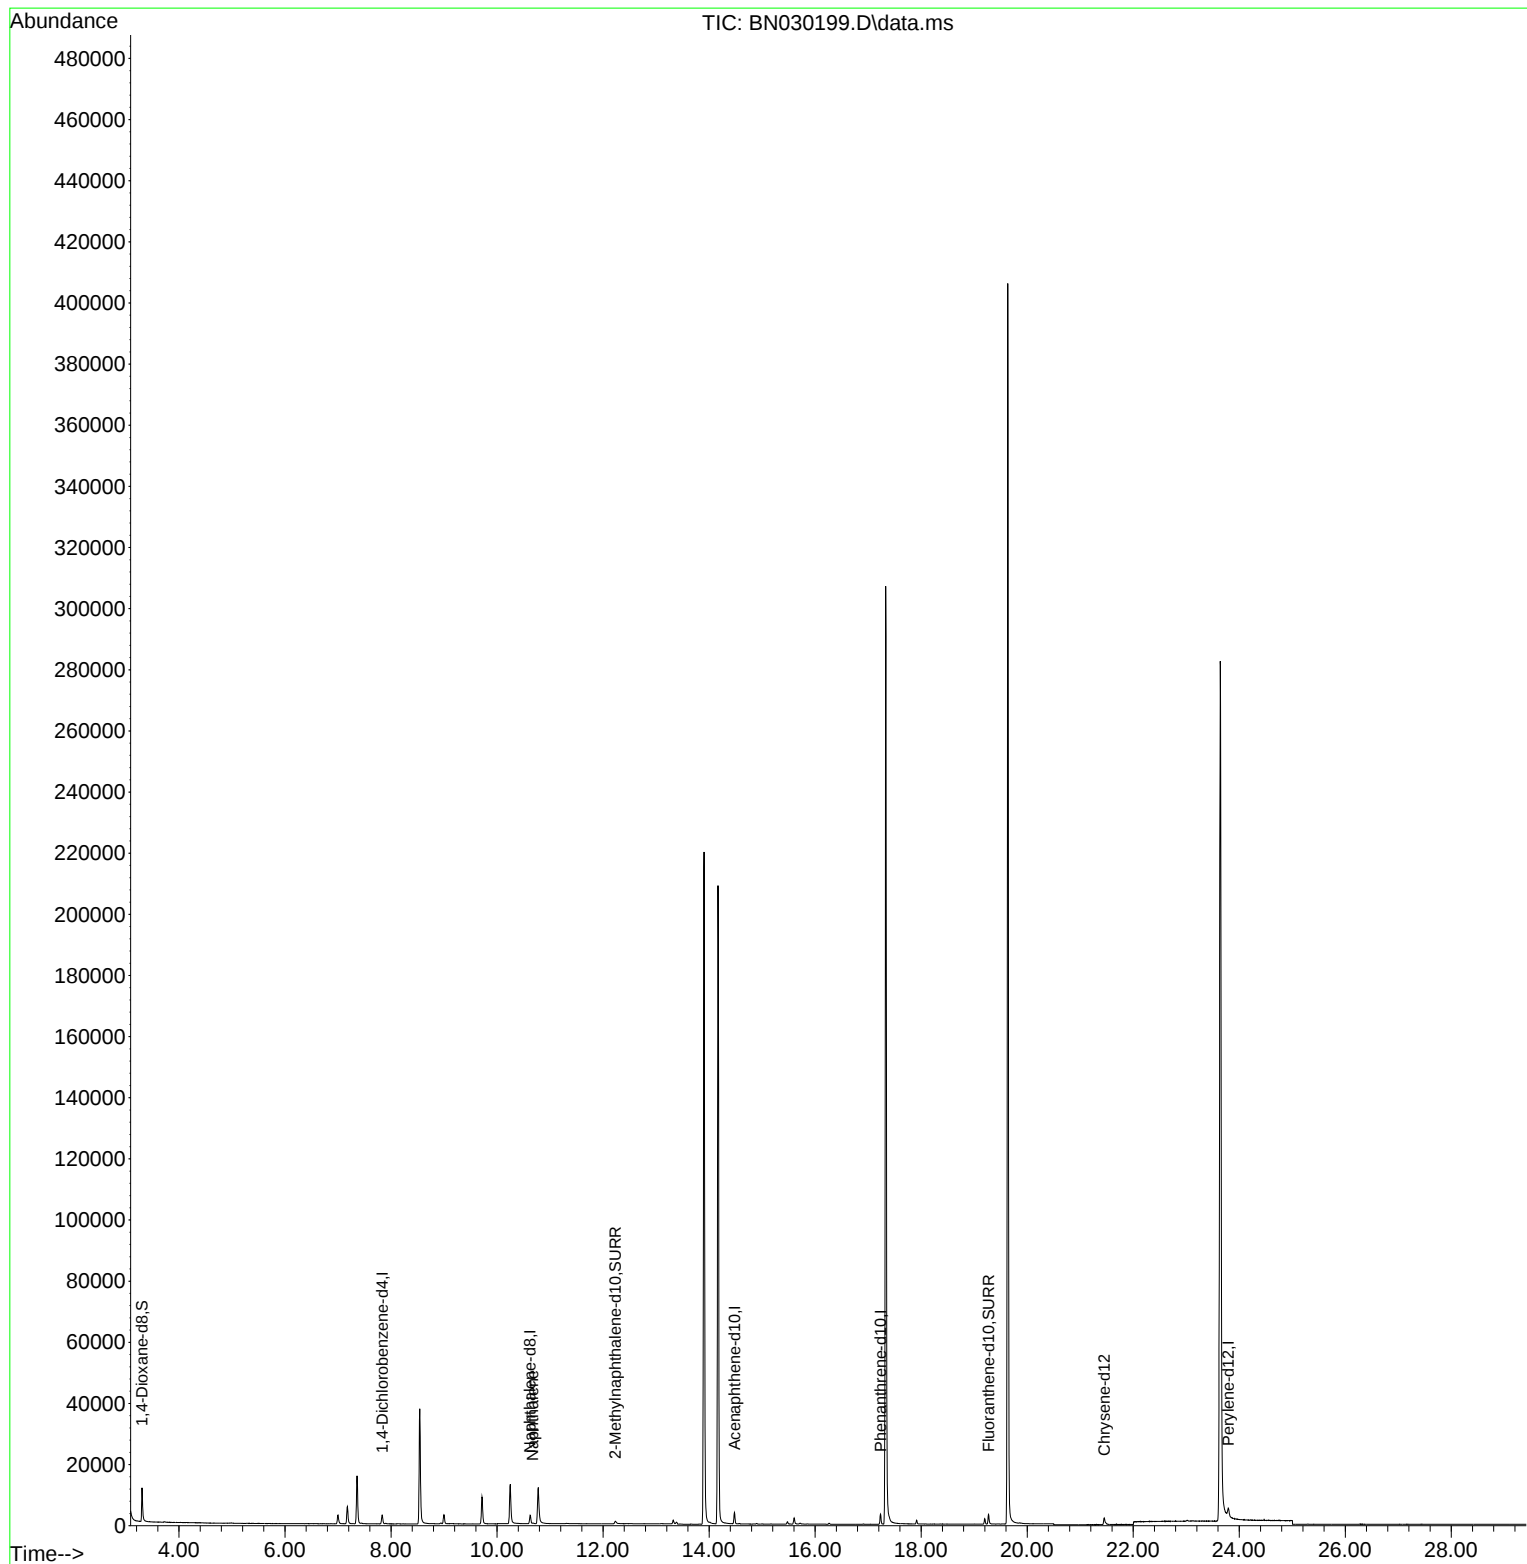

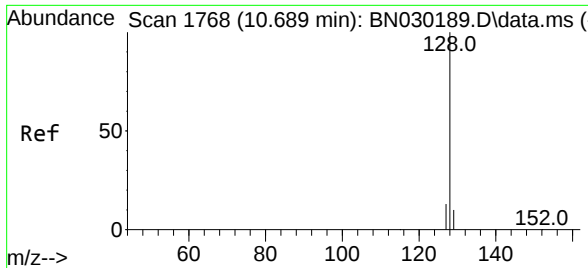

#5
Naphthalene
Concen: 0.021 ng/ul
RT: 10.672 min Scan# 1765
Delta R.T. -0.016 min
Lab File: BN030199.D
Acq: 03 Mar 2024 02:32

Instrument :
BNA_N
ClientSampleId :
E10B4

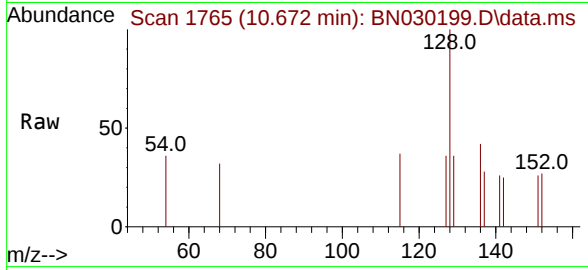

Tgt Ion:128 Resp: 250

Ion	Ratio	Lower	Upper
128	100		
129	35.7	11.0	16.4
127	35.7	12.3	18.5

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 03/04/2024
Supervised By :mohammad ahmed 03/05/2024

