

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
 Data File : BN030230.D
 Acq On : 03 Mar 2024 22:23
 Operator : MA/JU
 Sample : P1535-04
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AE7

Quant Time: Mar 03 22:55:28 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 02 16:09:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.830	152	1387	0.400	ng/ul	0.00
4) Naphthalene-d8	10.623	136	3767	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.474	164	1903	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.230	188	4096	0.400	ng/ul	#-0.02
17) Chrysene-d12	21.444	240	3860	0.400	ng/ul	# 0.00
23) Perylene-d12	23.791	264	6366	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.303	96	7605	3.961	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.229	152	1846	0.379	ng/ul	-0.01
18) Fluoranthene-d10	19.267	212	5380	0.428	ng/ul	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.340	88	1100	0.528	ng/ul	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
Data File : BN030230.D
Acq On : 03 Mar 2024 22:23
Operator : MA/JU
Sample : P1535-04
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AE7

Quant Time: Mar 03 22:55:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 02 16:09:30 2024
Response via : Initial Calibration

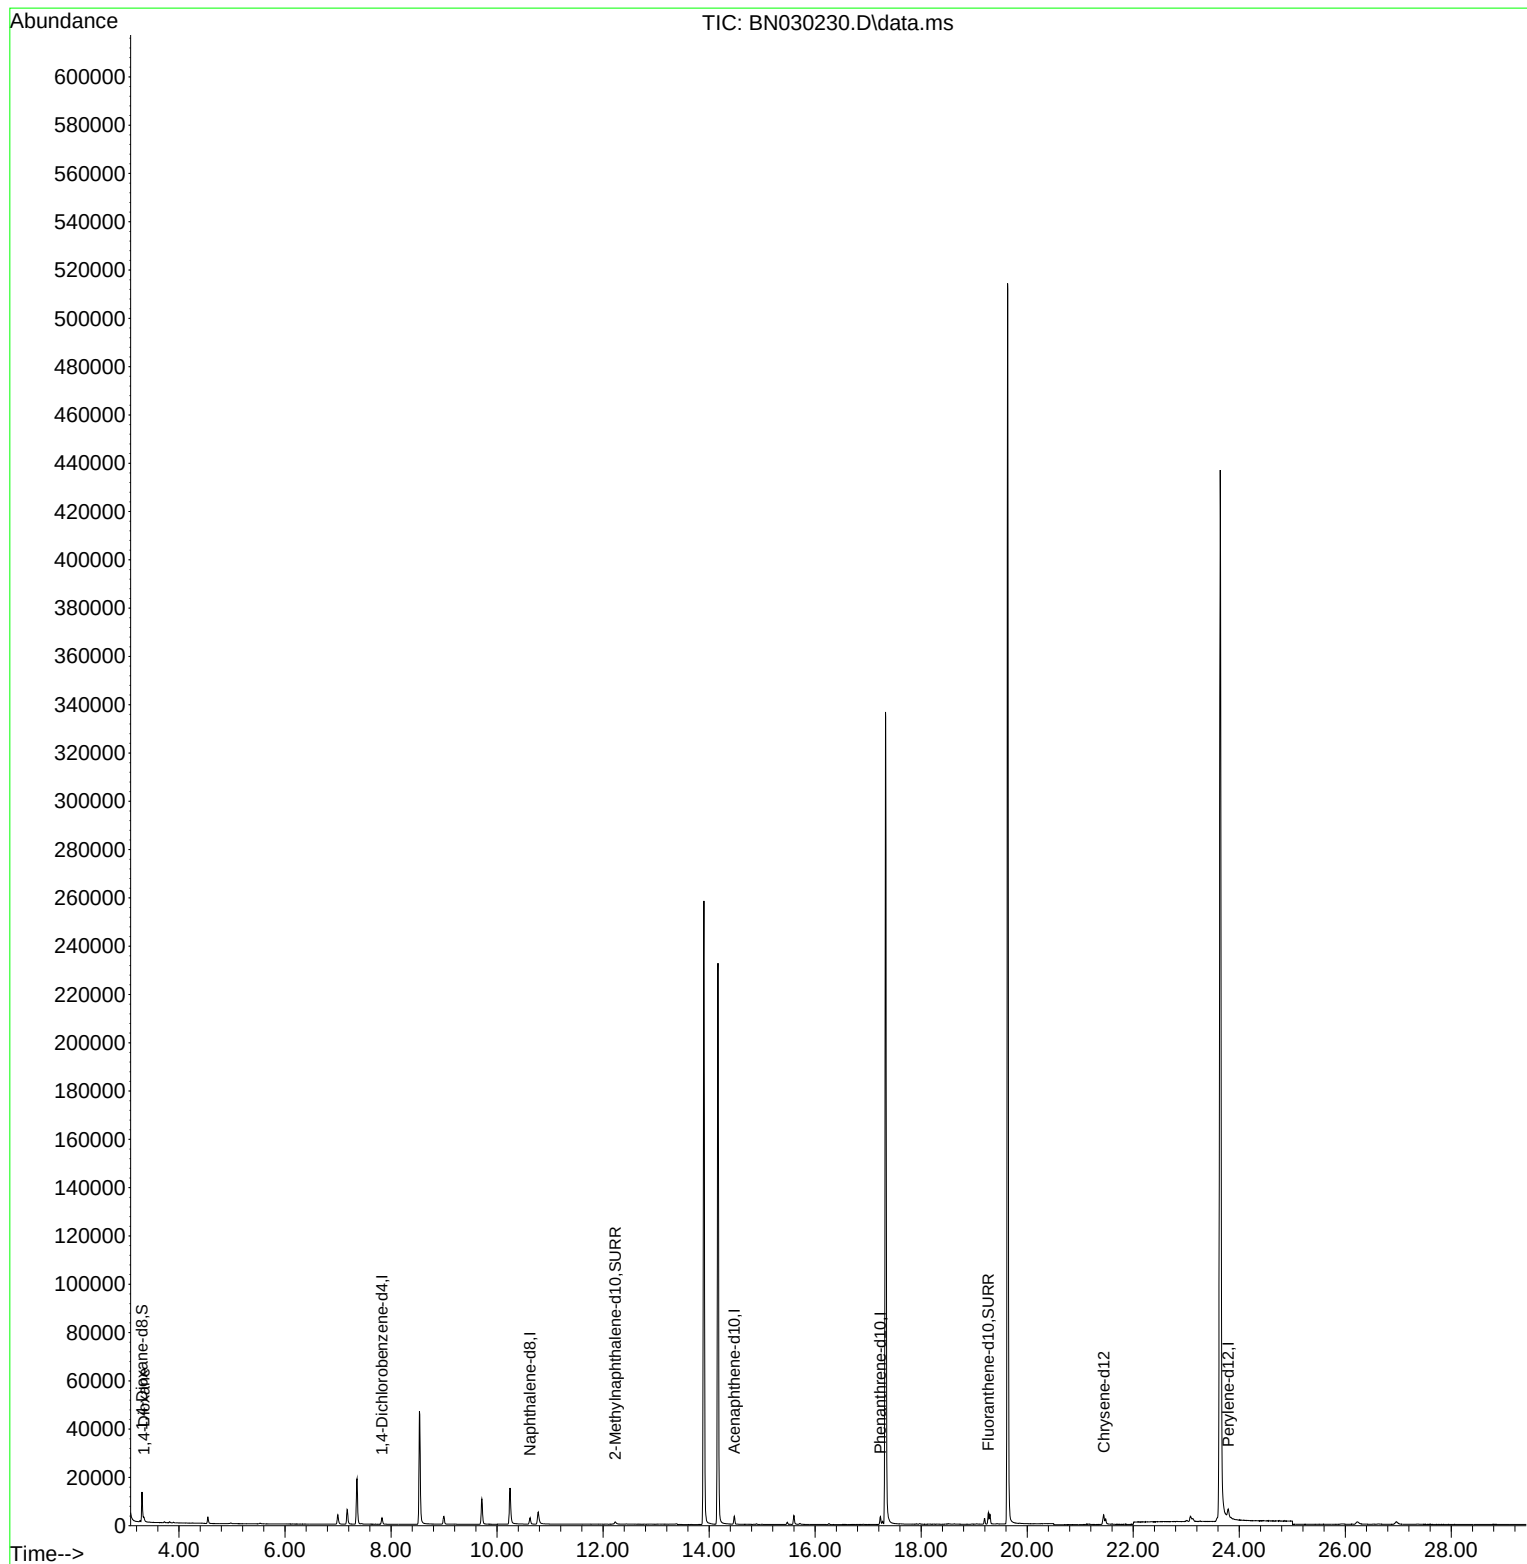

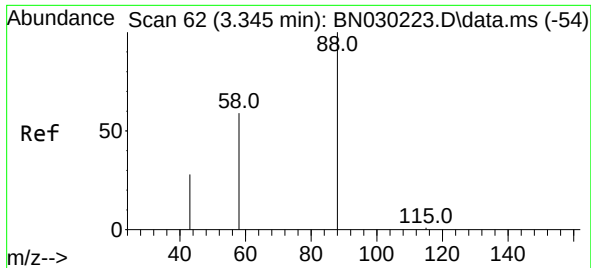

#2
 1,4-Dioxane
 Concen: 0.528 ng/ul
 RT: 3.340 min Scan# 61
 Delta R.T. 0.000 min
 Lab File: BN030230.D
 Acq: 03 Mar 2024 22:23

Instrument :
 BNA_N
 ClientSampleId :
 C0AE7

Tgt Ion: 88	Resp:	1100	
Ion	Ratio	Lower	Upper
88	100		
43	34.7	25.7	38.5
58	46.5	33.8	50.8

