

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
 Data File : BN030231.D
 Acq On : 03 Mar 2024 22:59
 Operator : MA/JU
 Sample : P1535-07
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AF4

Quant Time: Mar 03 23:59:10 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 02 16:09:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.829	152	1875	0.400	ng/ul	0.00
4) Naphthalene-d8	10.623	136	5114	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.474	164	2545	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.230	188	4965	0.400	ng/ul	#-0.02
17) Chrysene-d12	21.444	240	3594	0.400	ng/ul	# 0.00
23) Perylene-d12	23.788	264	5790	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.302	96	9860	3.799	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.228	152	3006	0.455	ng/ul	-0.01
18) Fluoranthene-d10	19.267	212	5896	0.504	ng/ul	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.340	88	2955	1.049	ng/ul#	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
Data File : BN030231.D
Acq On : 03 Mar 2024 22:59
Operator : MA/JU
Sample : P1535-07
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AF4

Quant Time: Mar 03 23:59:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 02 16:09:30 2024
Response via : Initial Calibration

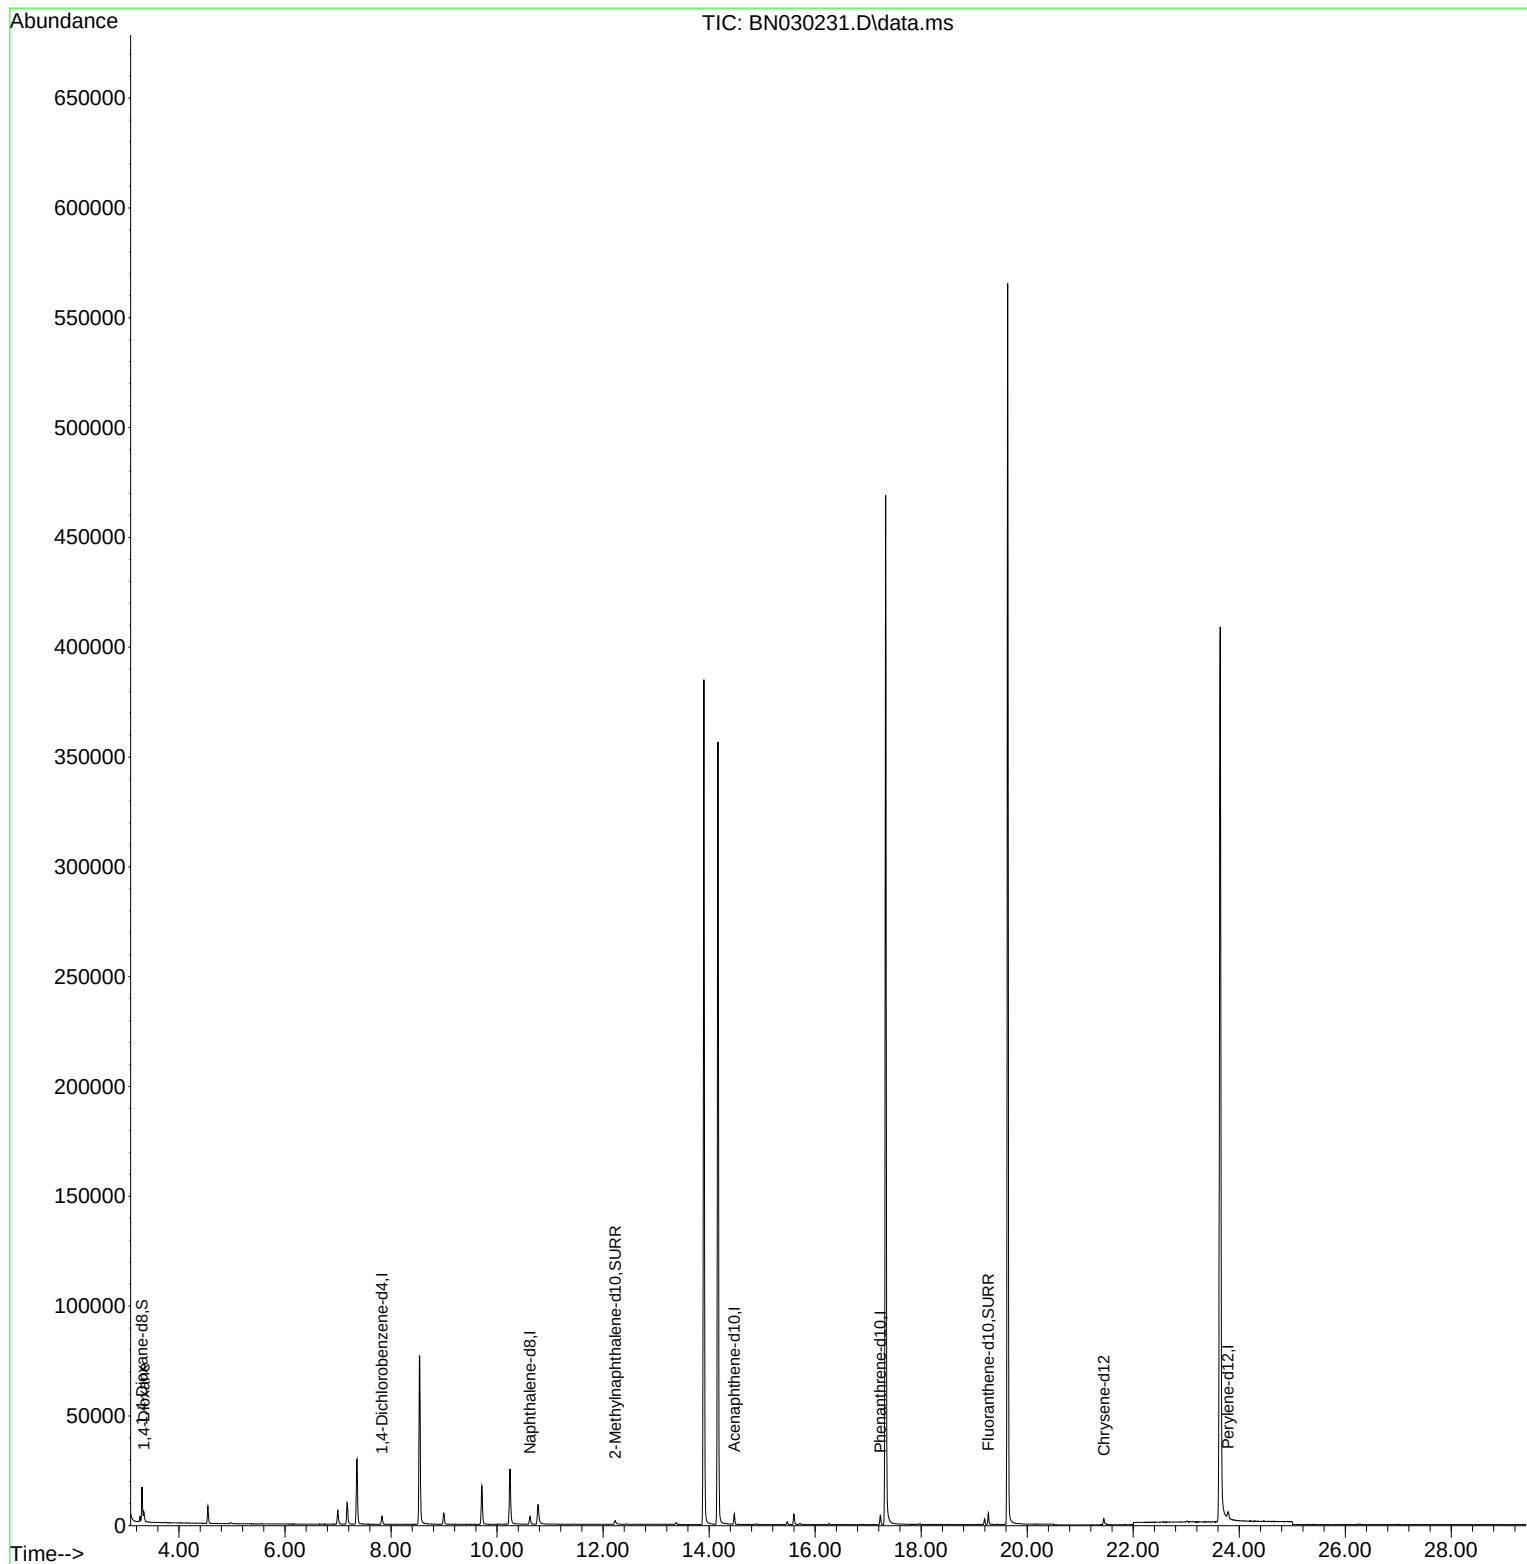

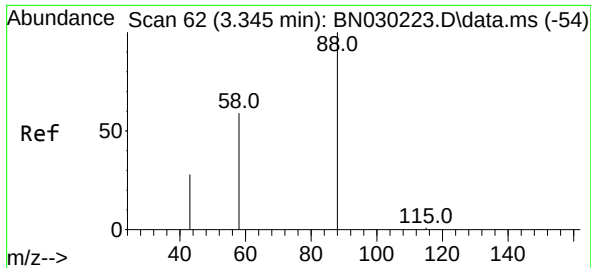

#2
 1,4-Dioxane
 Concen: 1.049 ng/ul
 RT: 3.340 min Scan# 61
 Delta R.T. 0.000 min
 Lab File: BN030231.D
 Acq: 03 Mar 2024 22:59

Instrument :
 BNA_N
 ClientSampleId :
 C0AF4

Tgt Ion: 88 Resp: 2955
 Ion Ratio Lower Upper
 88 100
 43 31.1 25.7 38.5
 58 53.0 33.8 50.8#

