

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
 Data File : BN030232.D
 Acq On : 03 Mar 2024 23:35
 Operator : MA/JU
 Sample : P1535-08
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AF5

Quant Time: Mar 04 00:12:32 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 02 16:09:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.830	152	1378	0.400	ng/ul	0.00
4) Naphthalene-d8	10.623	136	3694	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.474	164	1852	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.230	188	3789	0.400	ng/ul	#-0.02
17) Chrysene-d12	21.444	240	3233	0.400	ng/ul	# 0.00
23) Perylene-d12	23.788	264	5546	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.302	96	8764	4.594	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.223	152	2451	0.513	ng/ul	-0.02
18) Fluoranthene-d10	19.267	212	5339	0.507	ng/ul	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.340	88	431	0.208	ng/ul#	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030224\
Data File : BN030232.D
Acq On : 03 Mar 2024 23:35
Operator : MA/JU
Sample : P1535-08
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AF5

Quant Time: Mar 04 00:12:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN030224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 02 16:09:30 2024
Response via : Initial Calibration

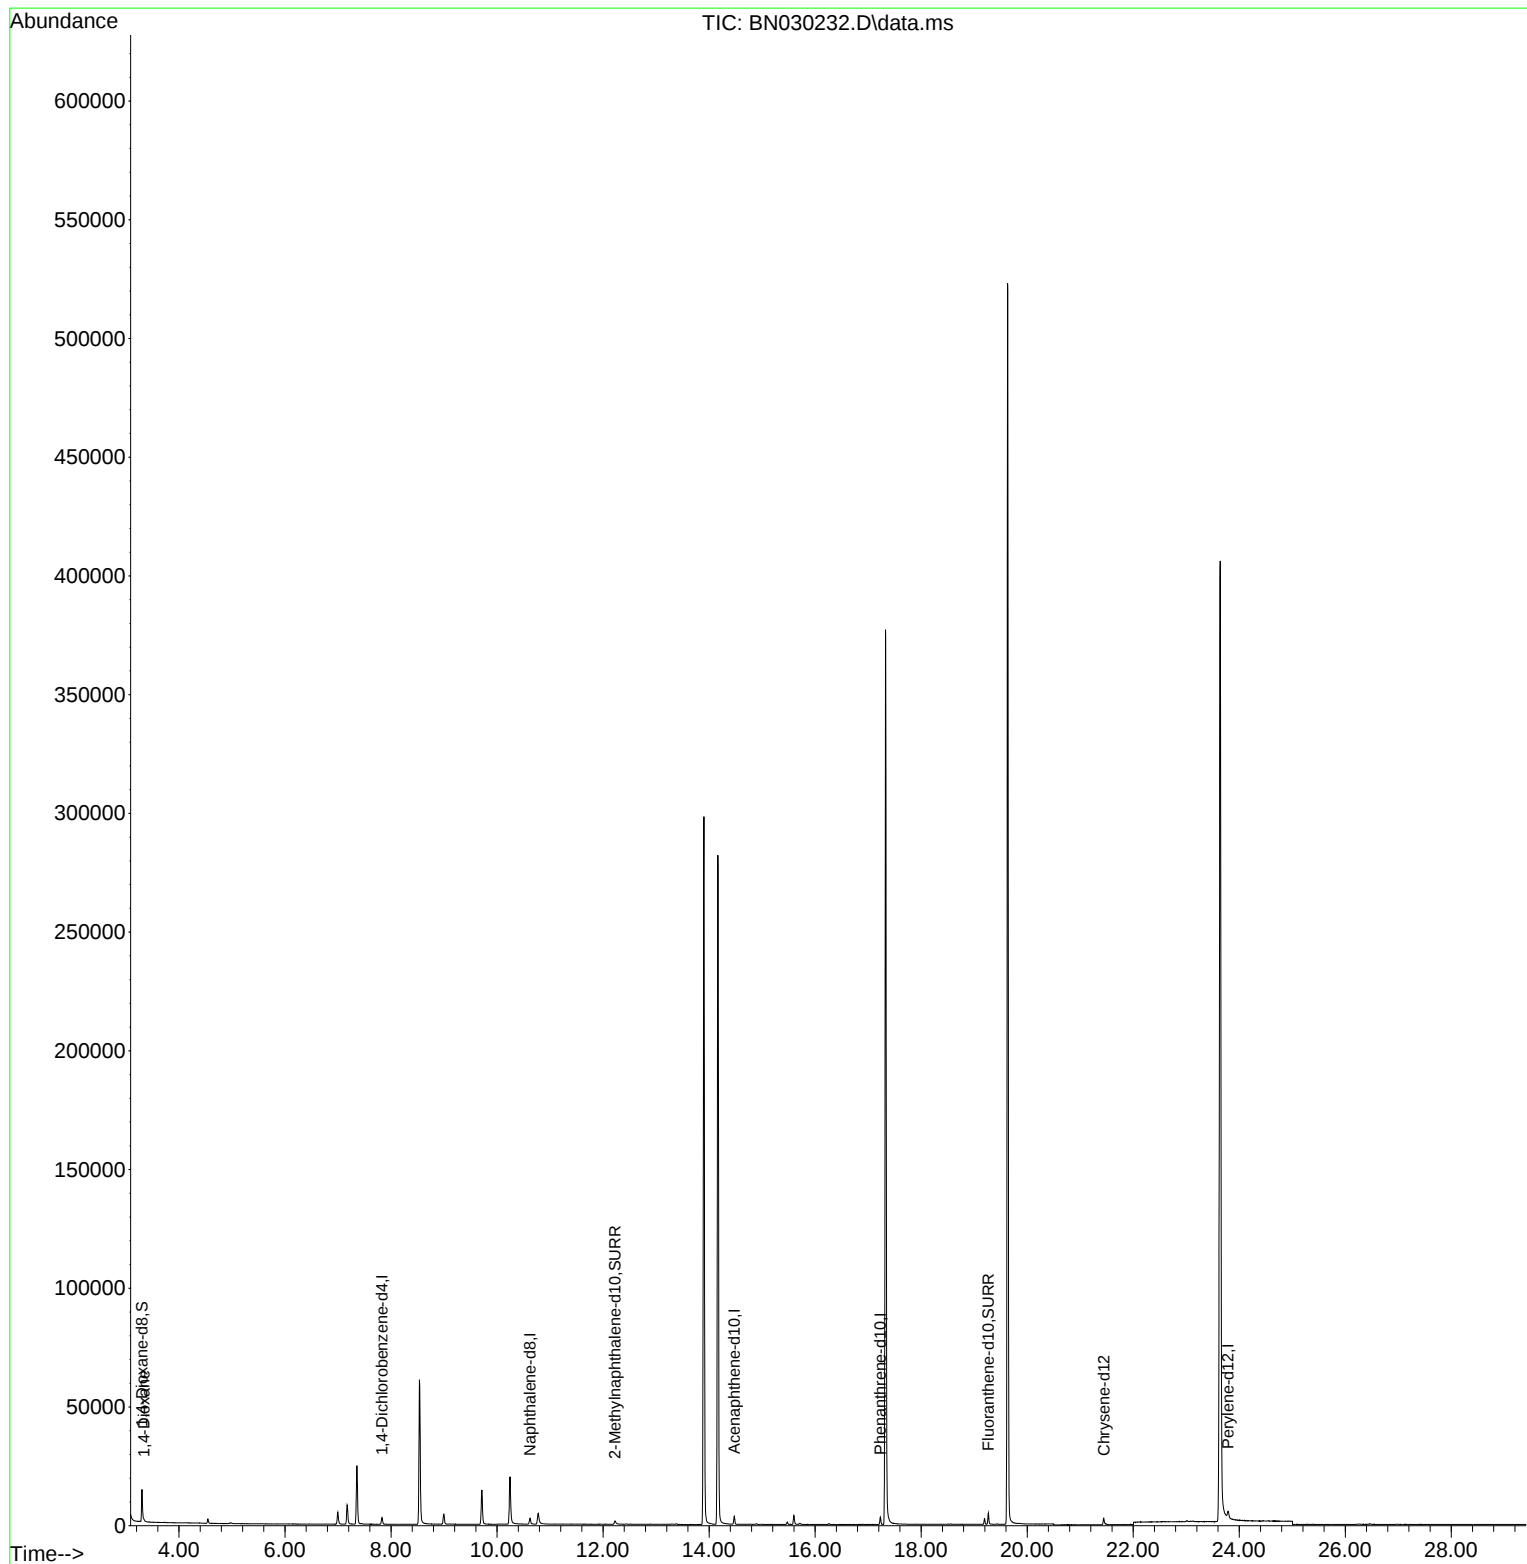

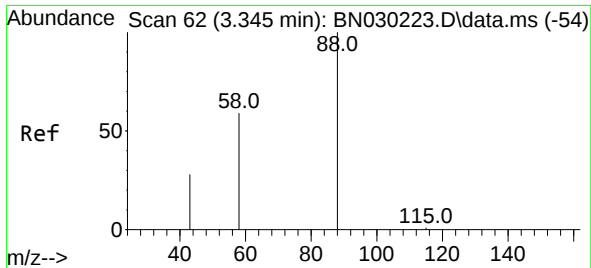

#2
 1,4-Dioxane
 Concen: 0.208 ng/ul
 RT: 3.340 min Scan# 61
 Delta R.T. 0.000 min
 Lab File: BN030232.D
 Acq: 03 Mar 2024 23:35

Instrument :
 BNA_N
 ClientSampleId :
 C0AF5

Tgt Ion: 88 Resp: 431
 Ion Ratio Lower Upper
 88 100
 43 40.6 25.7 38.5#
 58 36.7 33.8 50.8

