
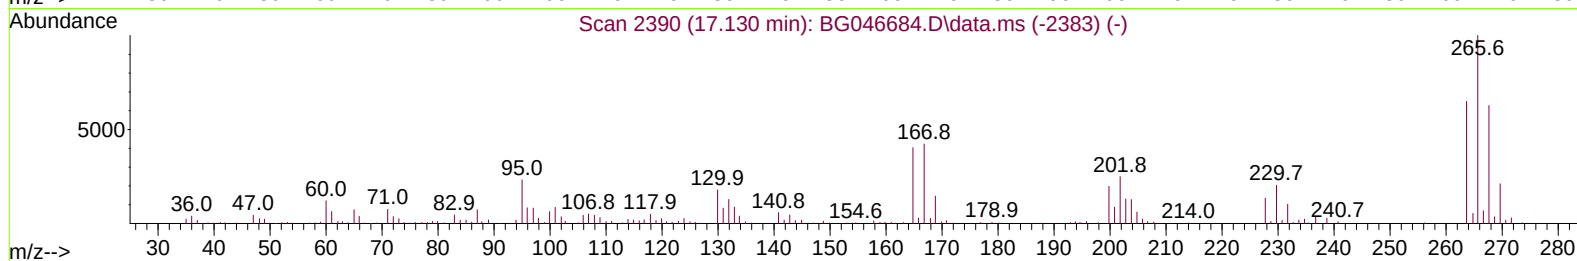
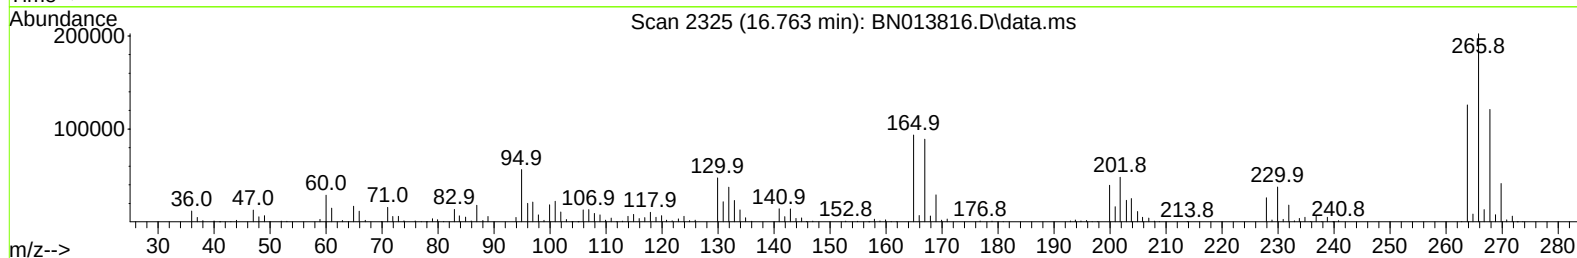


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030321\
Data File : BN013816.D
Acq On : 03 Mar 2021 11:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 04 08:37:25 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 26 07:31:37 2021
Response via : Initial Calibration

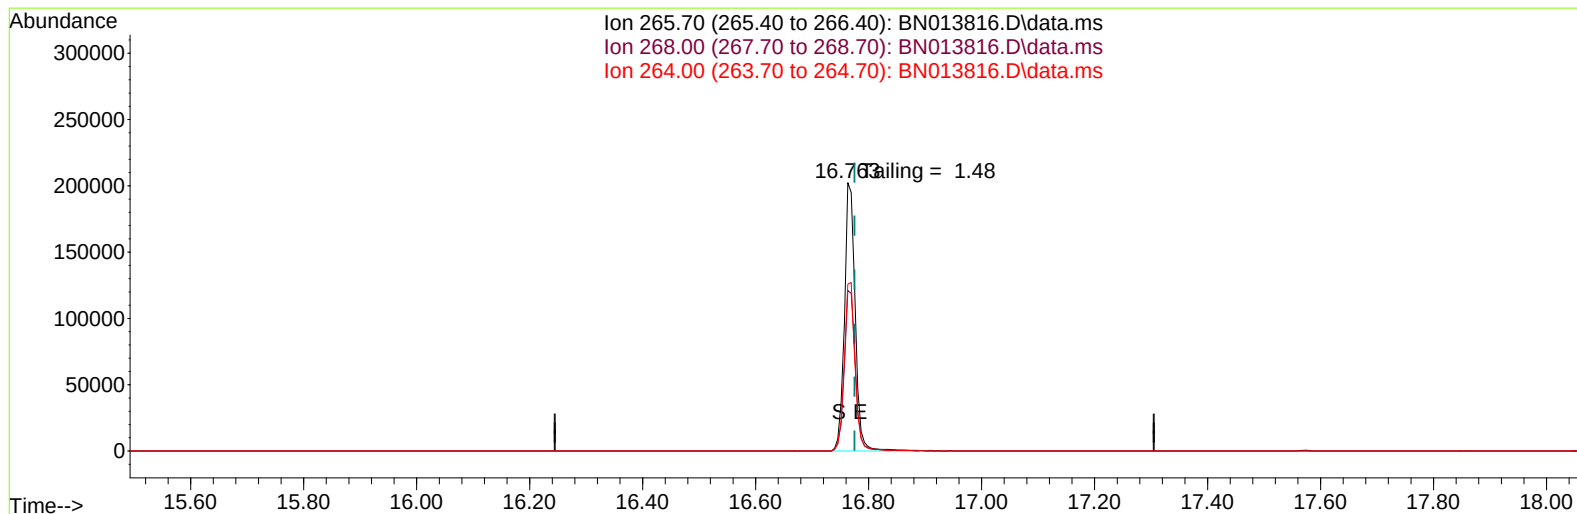

TIC: BN013816.D\data.ms

(70) Pentachlorophenol (C)




16.763min (-0.012) 22754.04 ng

response 266602

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.81
264.00	61.60	62.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030321\
 Data File : BN013816.D
 Acq On : 03 Mar 2021 11:03
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 04 08:37:25 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 26 07:31:37 2021
 Response via : Initial Calibration

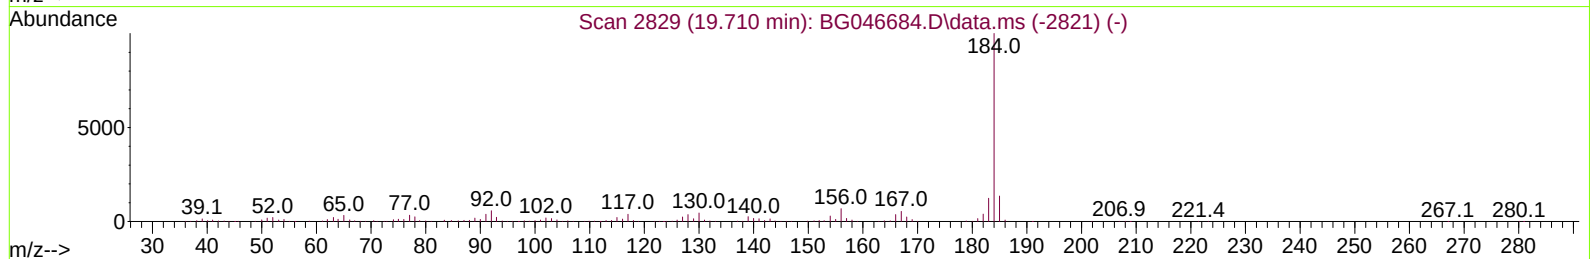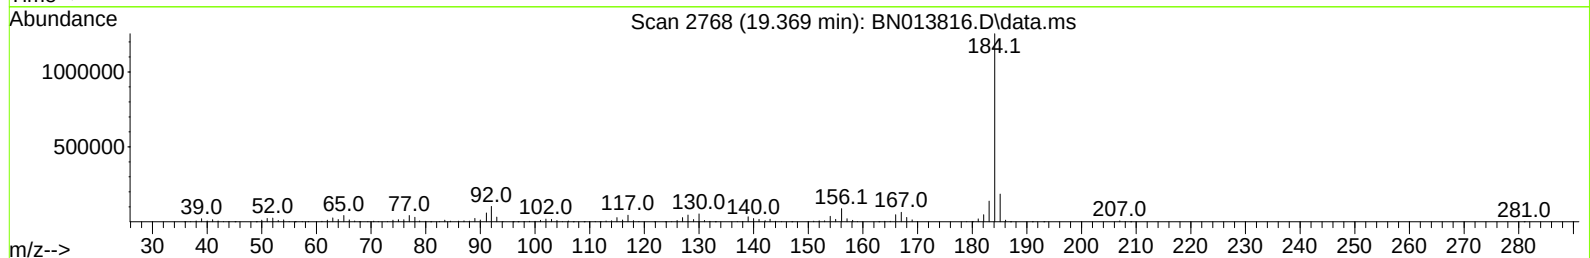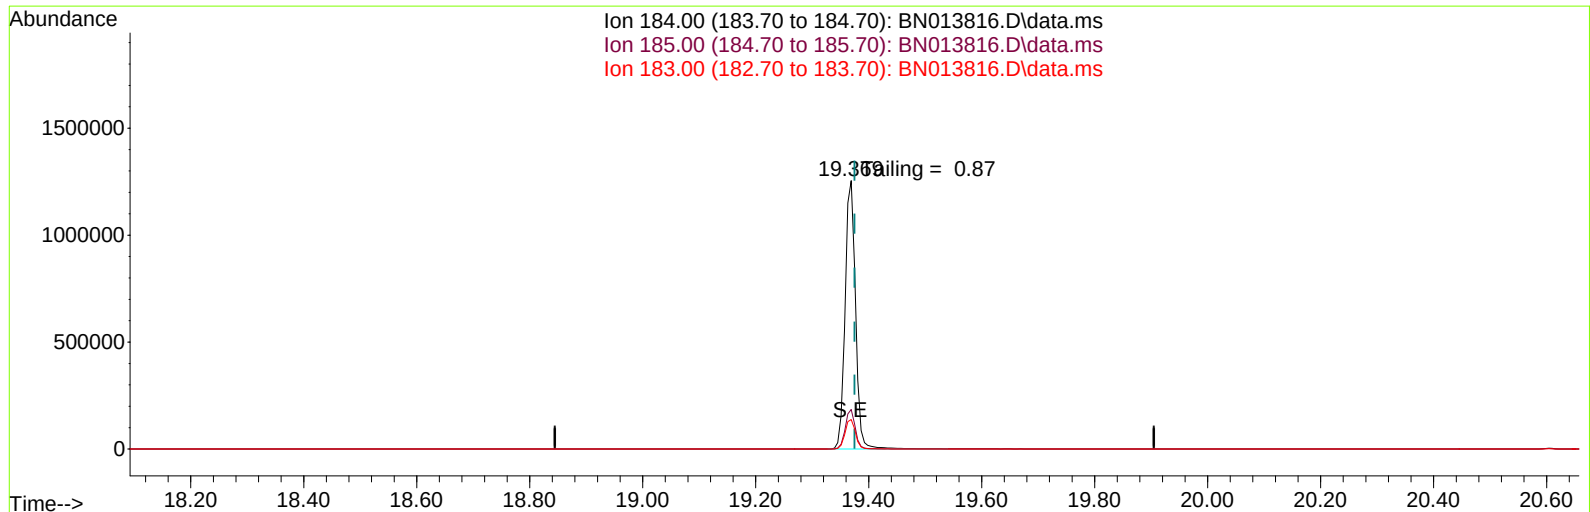

TIC: BN013816.D\data.ms

(77) Benzidine

19.369min (-0.006) 0.00 ng

response 1605098

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.72
183.00	13.20	10.97
0.00	0.00	0.00