


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030321\
 Data File : BN013816.D
 Acq On : 03 Mar 2021 11:03
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN022421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Feb 25 11:31:11 2021

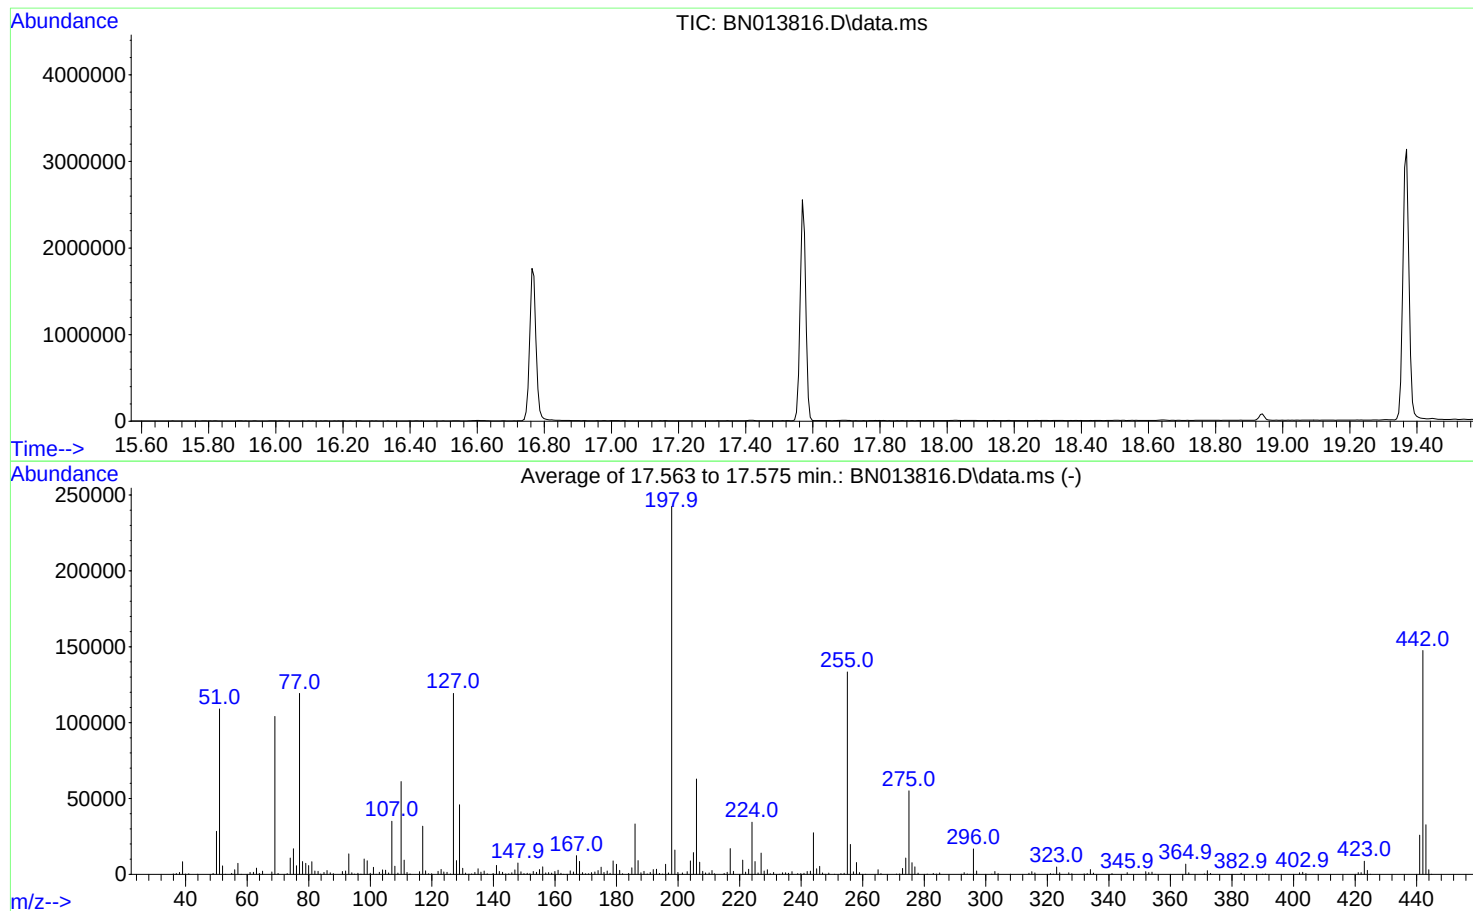




AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.0	109043	PASS
68	69	0.00	2	1.5	1569	PASS
69	198	0.00	100	42.9	104061	PASS
70	69	0.00	2	0.6	598	PASS
127	198	10	80	49.2	119293	PASS
197	198	0.00	2	0.4	985	PASS
198	198	100	100	100.0	242432	PASS
199	198	5	9	6.6	16013	PASS
275	198	10	60	22.7	55032	PASS
365	198	1	100	2.8	6789	PASS
441	198	0.01	100	10.7	25826	PASS
442	442	50	100	100.0	147544	PASS
443	442	15	24	22.2	32739	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030321\
Data File : BN013816.D
Acq On : 03 Mar 2021 11:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 04 08:37:25 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 26 07:31:37 2021
Response via : Initial Calibration

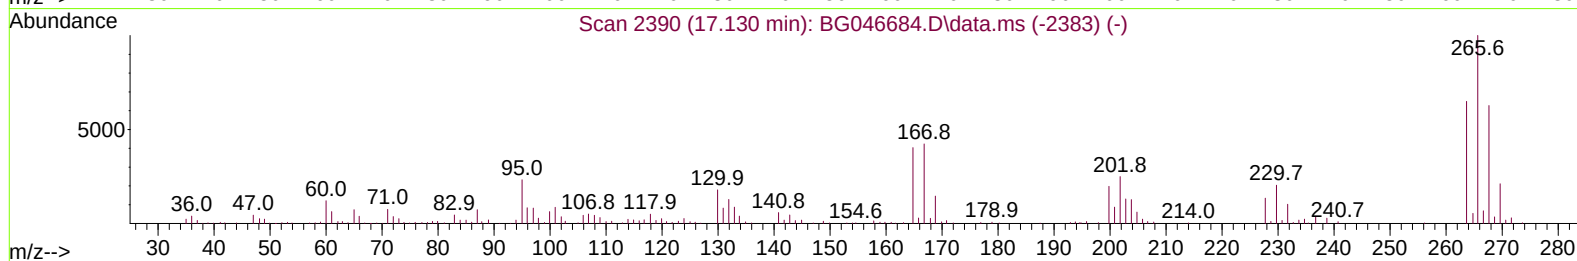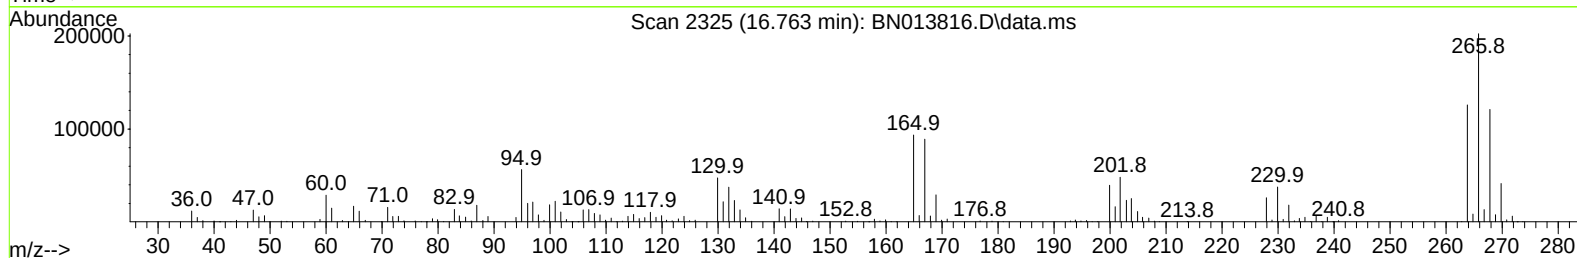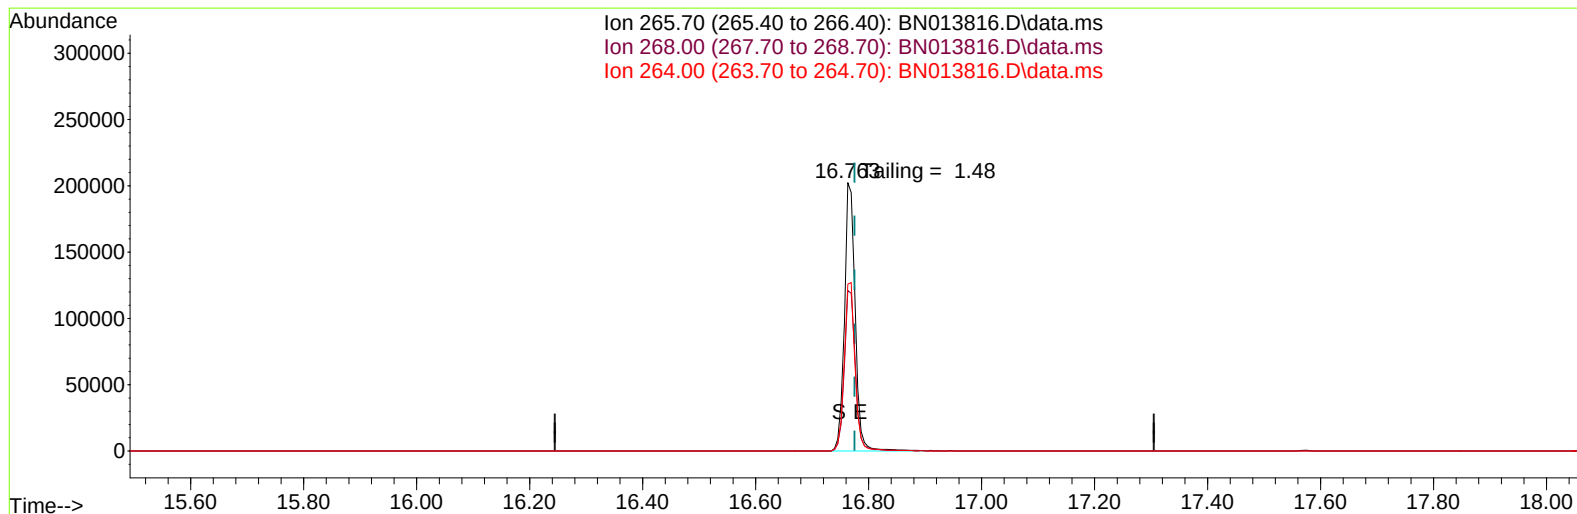

TIC: BN013816.D\data.ms

(70) Pentachlorophenol (C)

16.763min (-0.012) 22754.04 ng




response 266602

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.81
264.00	61.60	62.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030321\
Data File : BN013816.D
Acq On : 03 Mar 2021 11:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 04 08:37:25 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 26 07:31:37 2021
Response via : Initial Calibration

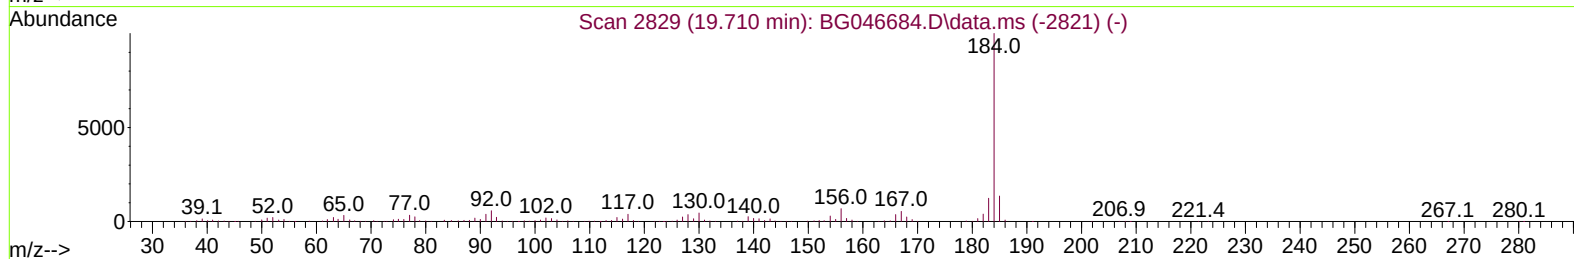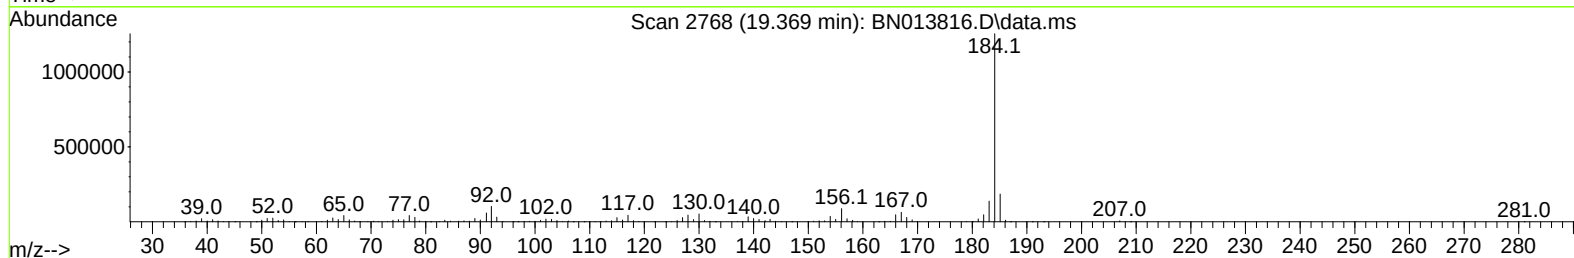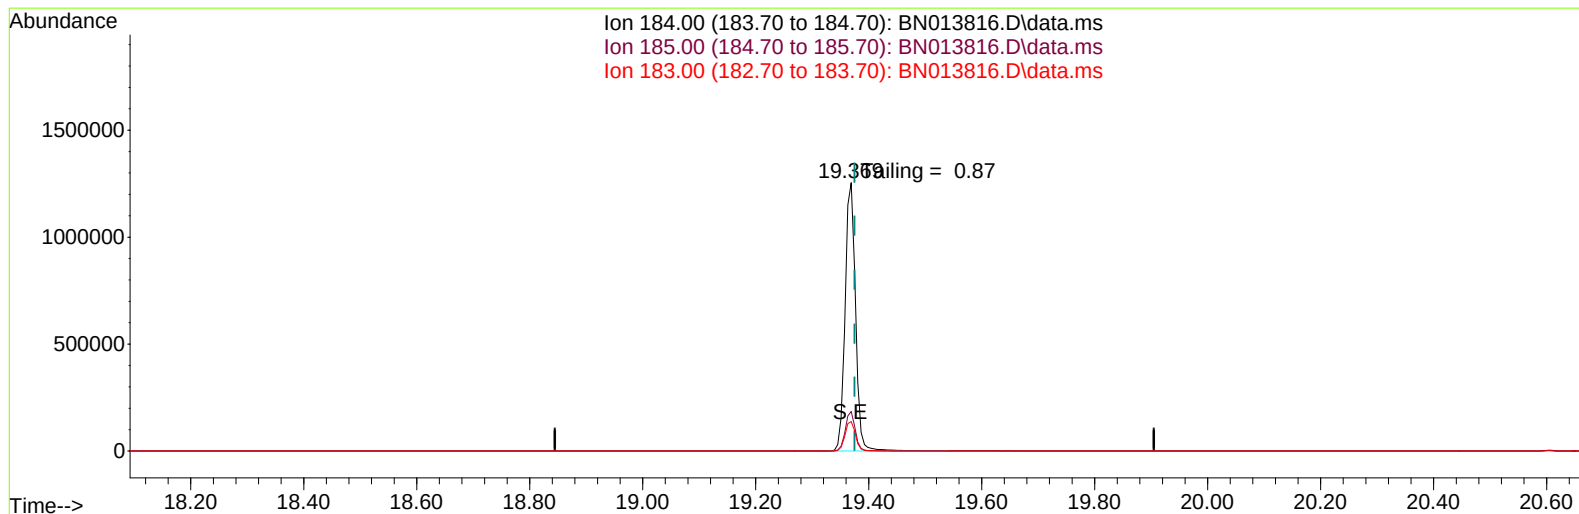

TIC: BN013816.D\data.ms

(77) Benzidine

19.369min (-0.006) 0.00 ng

response 1605098

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.72
183.00	13.20	10.97
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_N
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
3/3/2021	BNA_N	<u>BN013816.D</u>
Compound Name	Response	Retention Time
DDT	890602	20.6
DDD	10911	20.16
DDE	1937	19.65
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12848	903450	1.42