


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030322\
 Data File : BN018792.D
 Acq On : 02 Mar 2022 15:27
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN030322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 03 00:44:34 2022

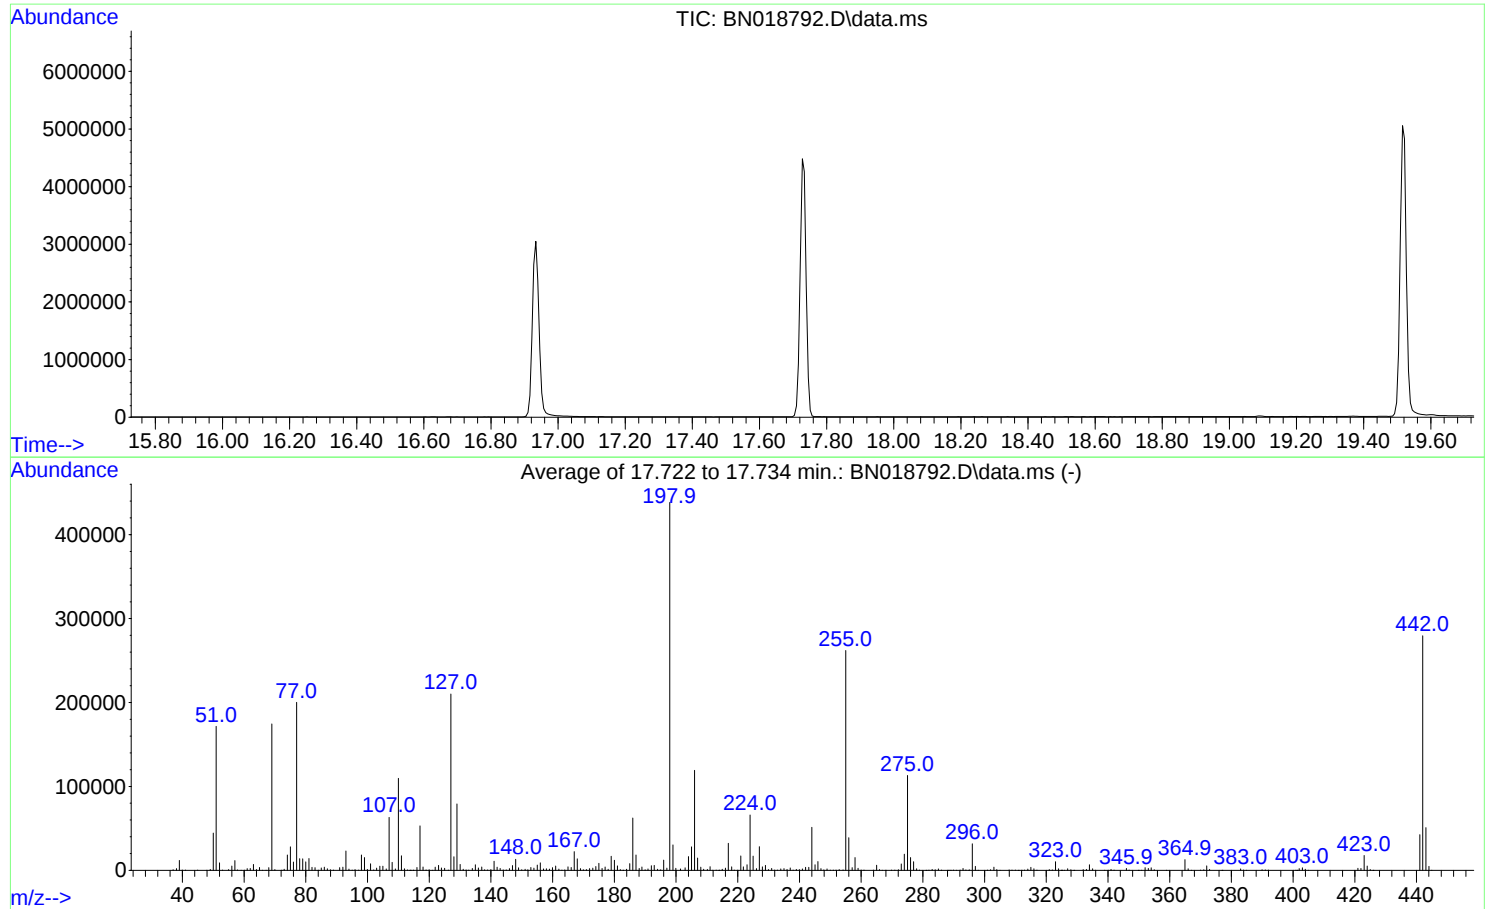

AutoFind: Scans 2505, 2506, 2507; Background Corrected with Scan 2498

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.1	171562	PASS
68	69	0.00	2	1.8	3223	PASS
69	198	0.00	100	39.8	174464	PASS
70	69	0.00	2	0.5	885	PASS
127	198	10	80	47.9	210133	PASS
197	198	0.00	2	0.6	2774	PASS
198	198	100	100	100.0	438315	PASS
199	198	5	9	6.9	30309	PASS
275	198	10	60	25.8	112997	PASS
365	198	1	100	2.9	12719	PASS
441	198	0.01	100	9.7	42557	PASS
442	442	50	100	100.0	279416	PASS
443	442	15	24	18.2	50947	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/3/2022	BNA_N	<u>BN018792.D</u>
Compound Name	Response	Retention Time
DDT	1525208	20.757
DDD	25408	20.316
DDE	825	19.81
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
26233	1551441	1.69

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030322\
 Data File : BN018792.D
 Acq On : 02 Mar 2022 15:27
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Mar 03 03:47:20 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 03 03:47:13 2022
 Response via : Initial Calibration

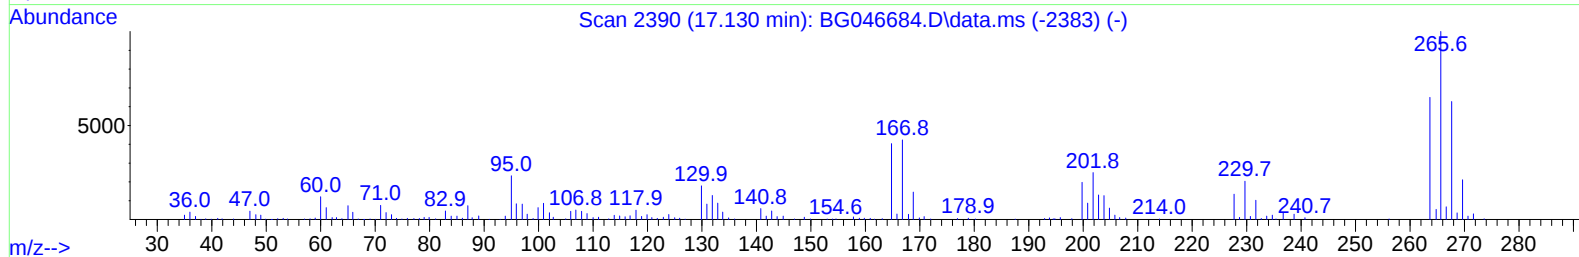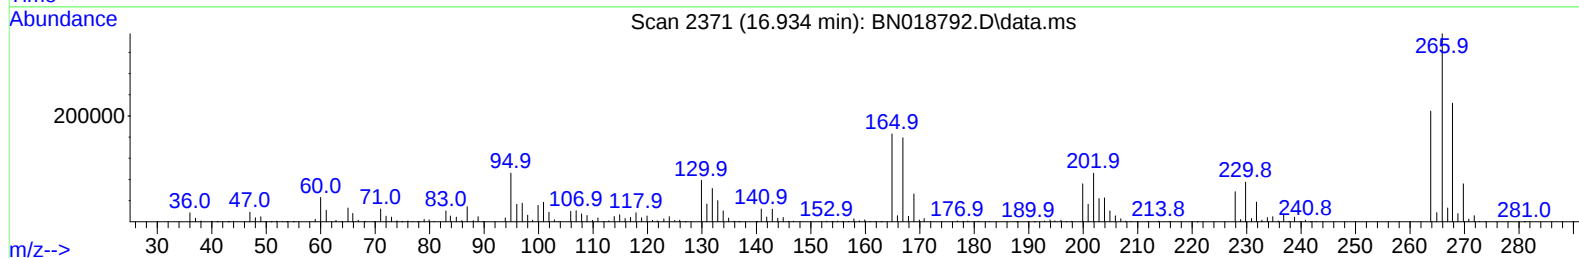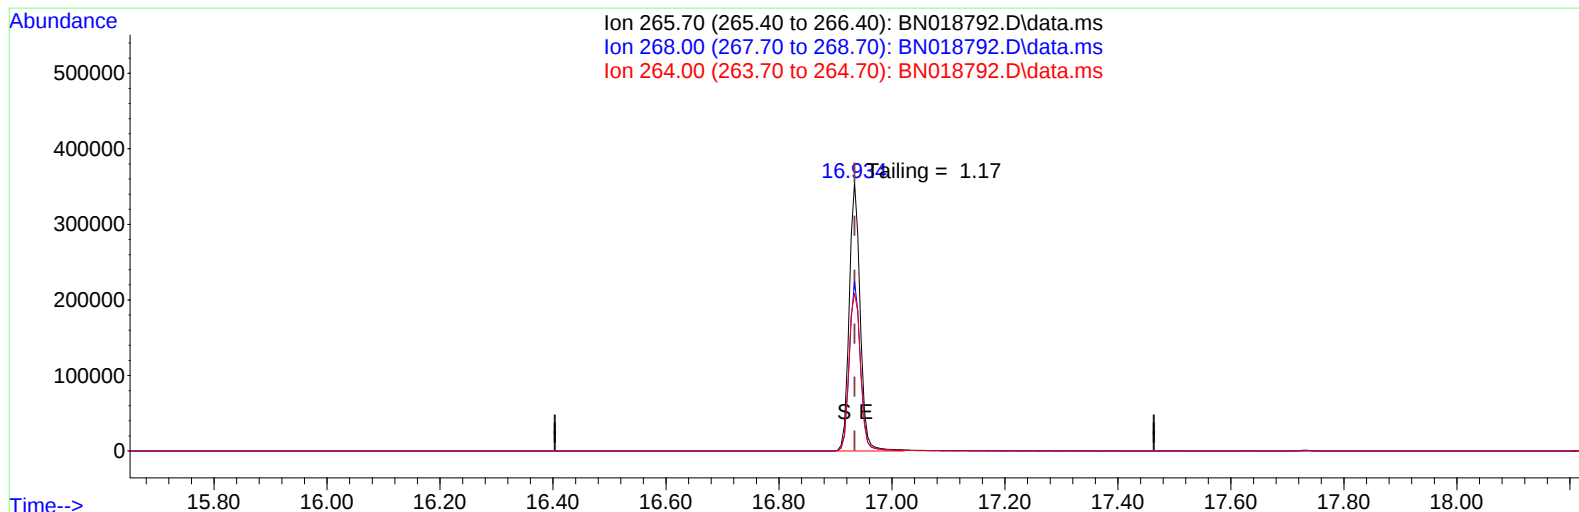

TIC: BN018792.D\data.ms

(70) Pentachlorophenol (C)

16.934min (0.000) 19538.47 ng




response 482999

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.11
264.00	61.60	58.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030322\
Data File : BN018792.D
Acq On : 02 Mar 2022 15:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 03 03:47:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 03 03:47:13 2022
Response via : Initial Calibration

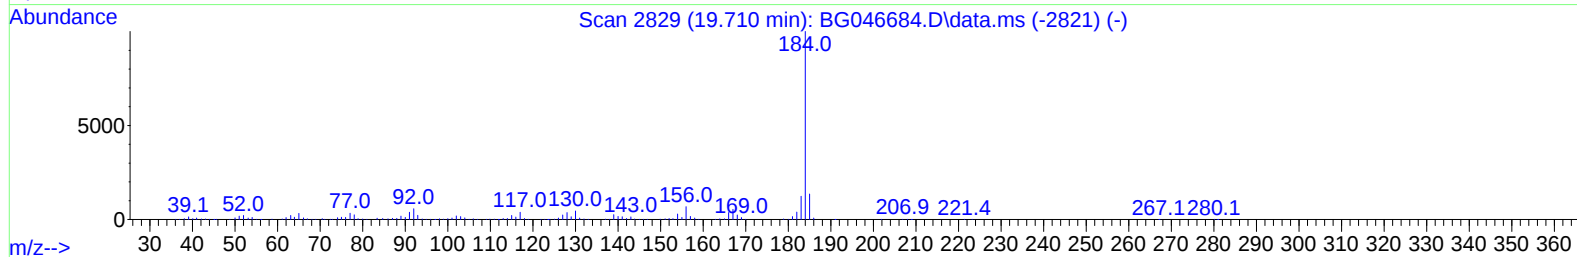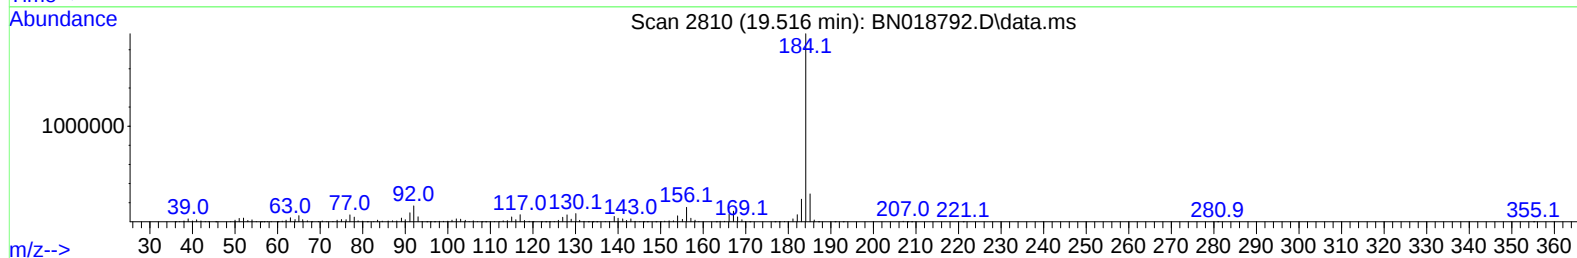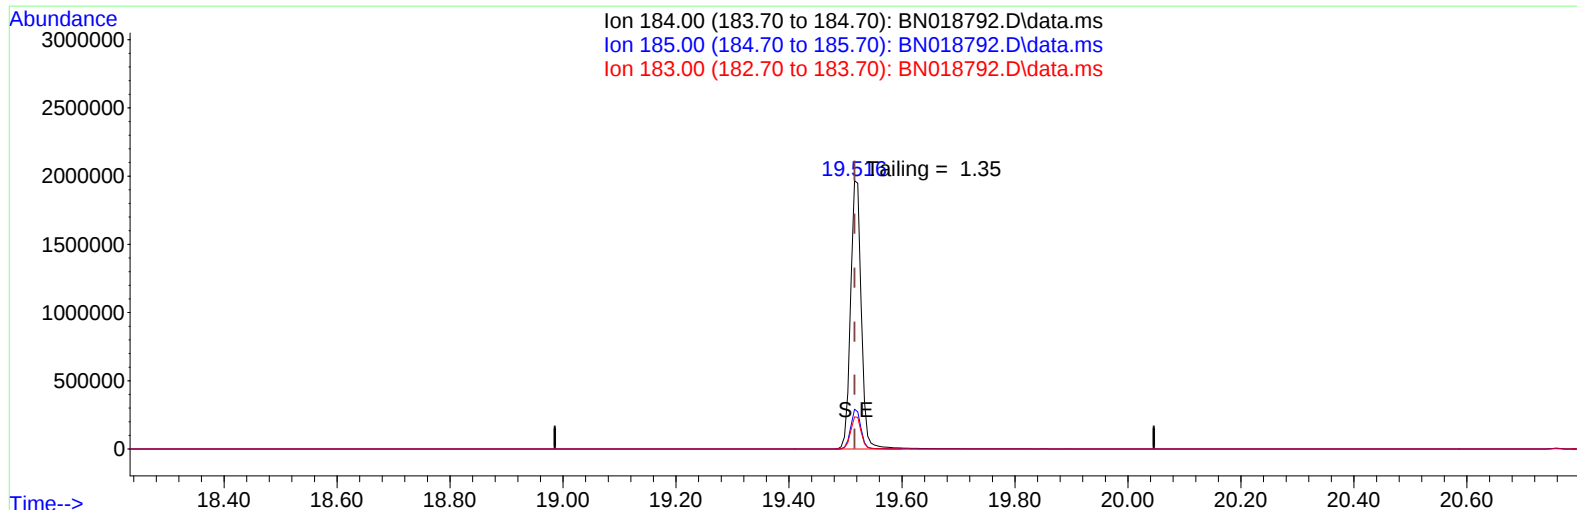

TIC: BN018792.D\data.ms

(77) Benzdine

19.516min (0.000) 0.00 ng

response 2629070

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.86
183.00	13.20	12.01
0.00	0.00	0.00