
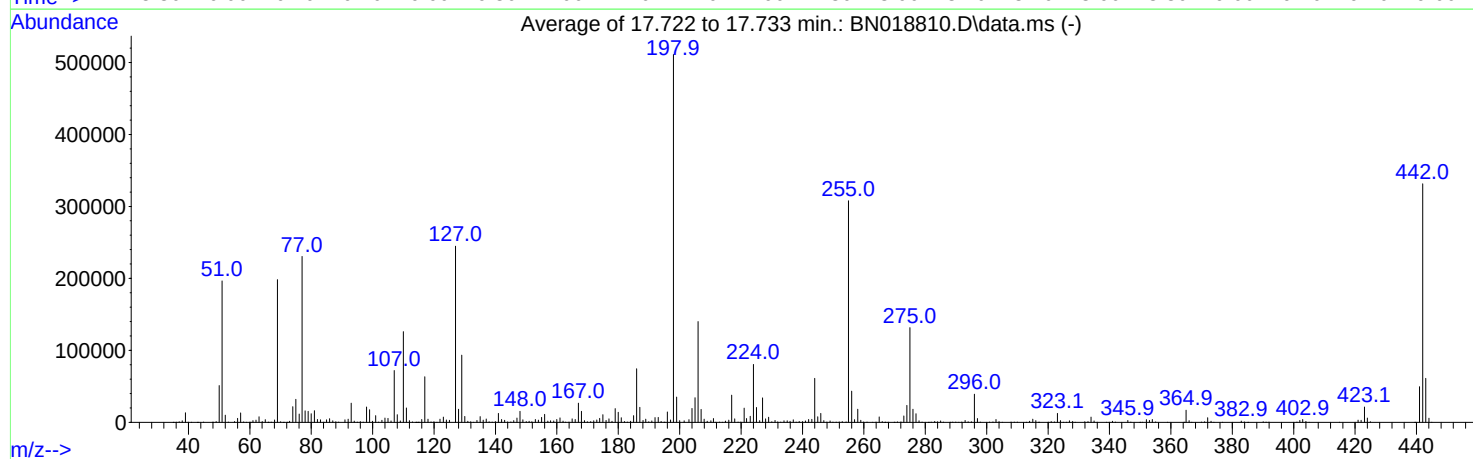


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030322\
 Data File : BN018810.D
 Acq On : 03 Mar 2022 04:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN030322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 03 00:44:34 2022

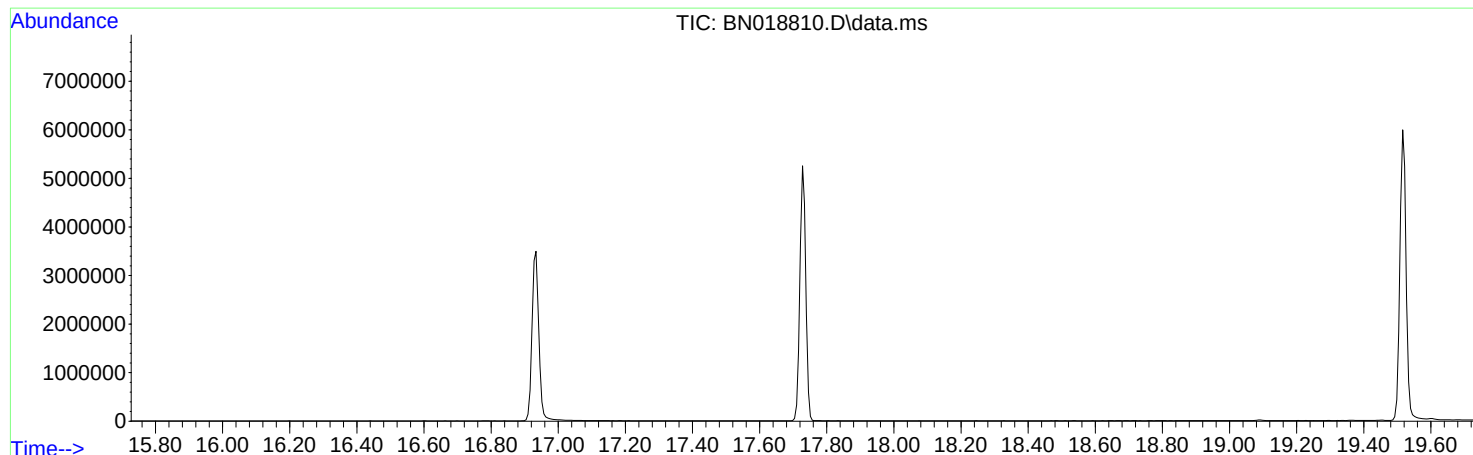




AutoFind: Scans 2505, 2506, 2507; Background Corrected with Scan 2498

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.4	196456	PASS
68	69	0.00	2	1.7	3431	PASS
69	198	0.00	100	38.8	198336	PASS
70	69	0.00	2	0.5	1013	PASS
127	198	10	80	47.9	244779	PASS
197	198	0.00	2	0.7	3380	PASS
198	198	100	100	100.0	511104	PASS
199	198	5	9	6.9	35245	PASS
275	198	10	60	25.8	131675	PASS
365	198	1	100	3.3	16943	PASS
441	198	0.01	100	9.7	49493	PASS
442	442	50	100	100.0	331520	PASS
443	442	15	24	18.5	61261	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030322\
Data File : BN018810.D
Acq On : 03 Mar 2022 04:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 03 05:03:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 03 05:03:14 2022
Response via : Initial Calibration

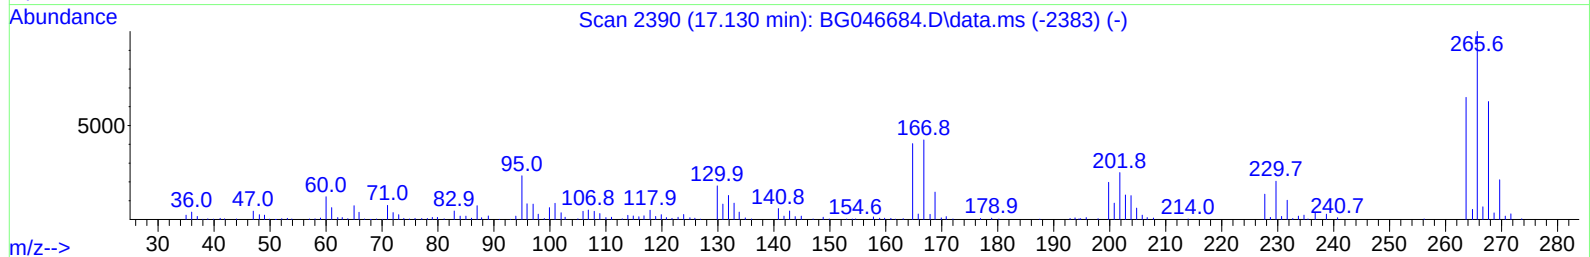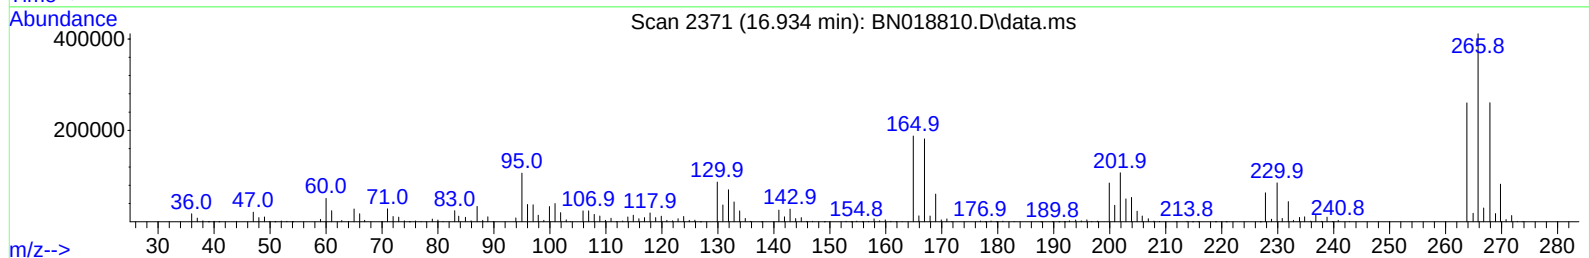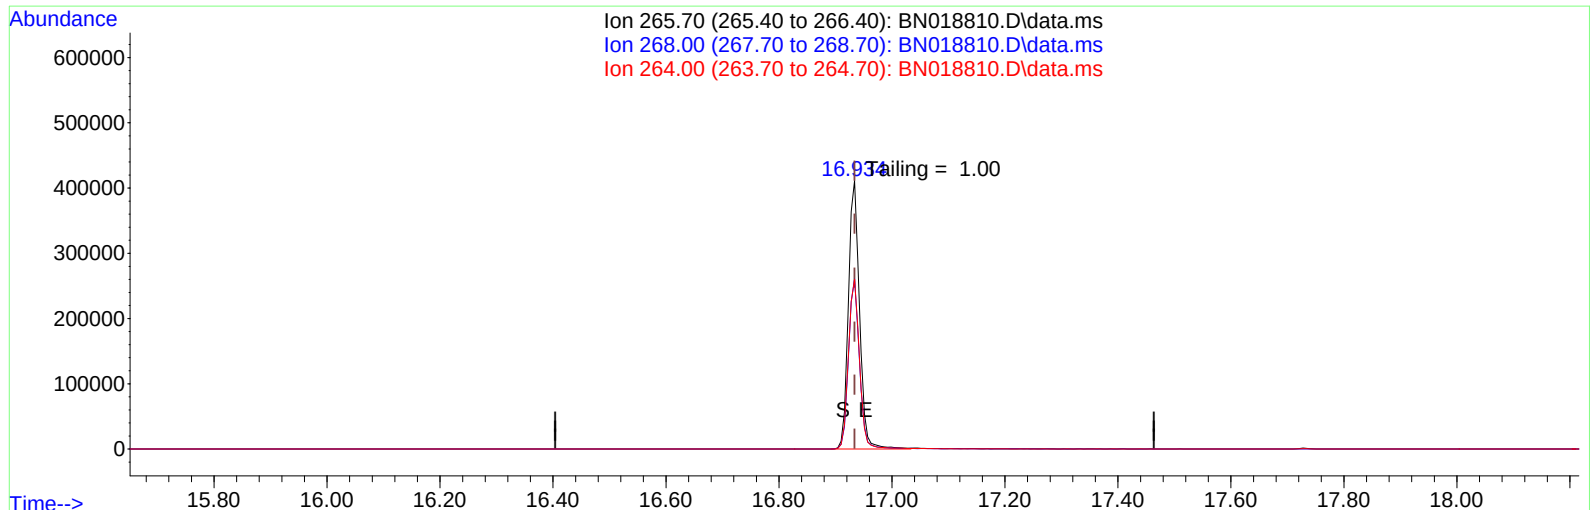

TIC: BN018810.D\data.ms

(70) Pentachlorophenol (C)

16.934min (0.000) 18659.76 ng




response 564515

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.33
264.00	61.60	63.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030322\
Data File : BN018810.D
Acq On : 03 Mar 2022 04:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 03 05:03:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 03 05:03:14 2022
Response via : Initial Calibration

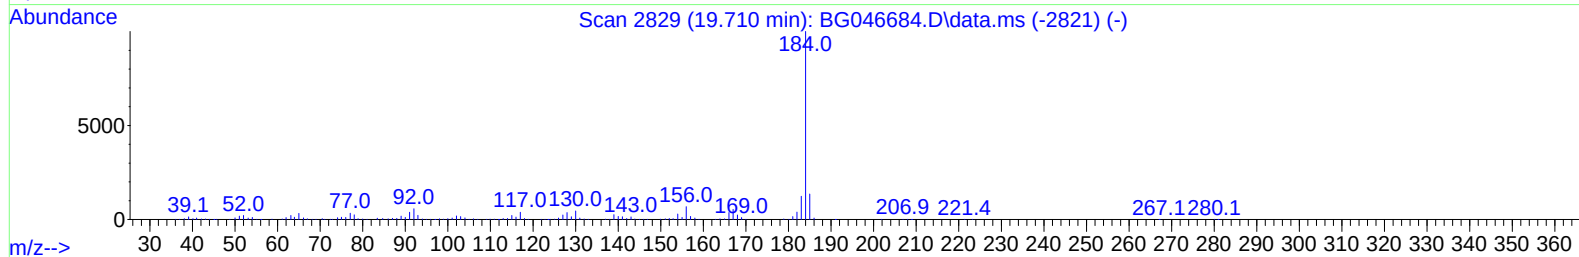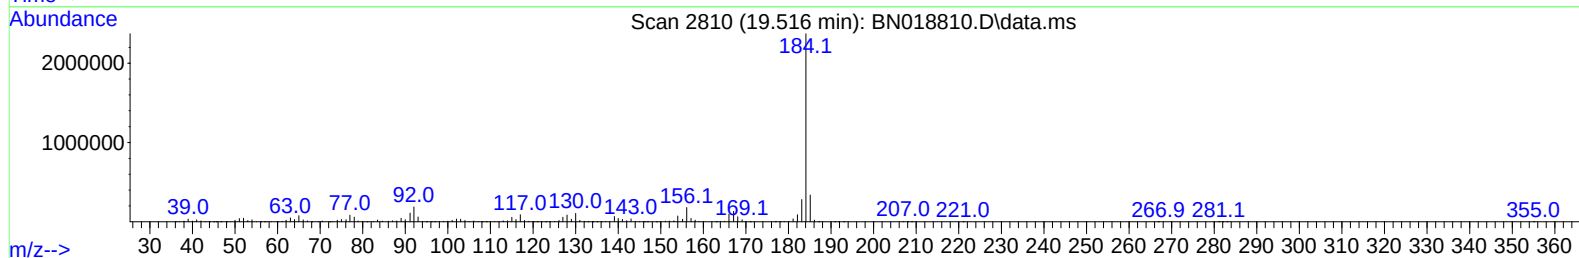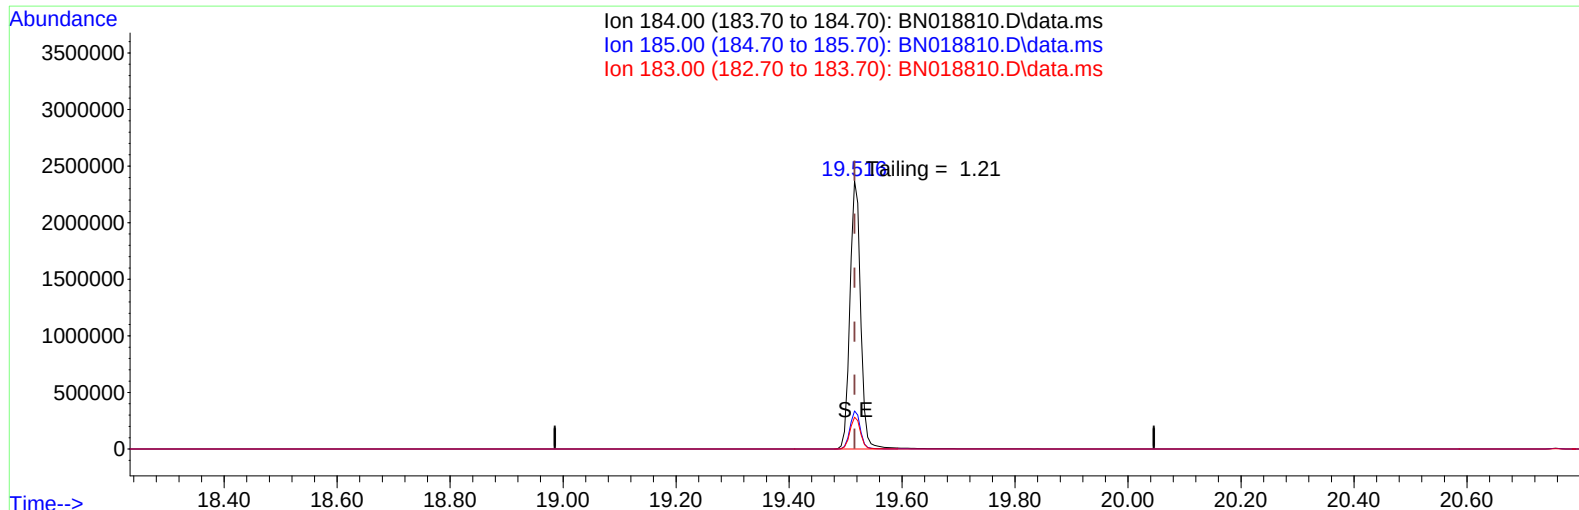

TIC: BN018810.D\data.ms

(77) Benzidine

19.516min (0.000) 0.00 ng

response 3153019

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.20
183.00	13.20	11.87
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/3/2022	BNA_N	<u>BN018810.D</u>
Compound Name	Response	Retention Time
DDT	1769926	20.757
DDD	40528	20.316
DDE	1438	19.81
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
41966	1811892	2.32