

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030422\
 Data File : BN018822.D
 Acq On : 03 Mar 2022 12:49
 Operator : CG/JU
 Sample : N1745-05
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 H0AA5

Quant Time: Mar 04 01:45:56 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN021822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 18 13:39:55 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.913	152	7042	0.400	ng/ul	0.00
4) Naphthalene-d8	10.715	136	20564	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.543	164	13283	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.284	188	29669	0.400	ng/ul	0.00
17) Chrysene-d12	21.463	240	23876	0.400	ng/ul	# 0.00
23) Perylene-d12	23.860	264	20496	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.280	96	39440	4.931	ng/ul	-0.02
6) 2-Methylnaphthalene-d10	12.305	152	10513	0.374	ng/ul	0.00
18) Fluoranthene-d10	19.309	212	33693	0.472	ng/ul	0.00
Target Compounds						
					Qvalue	
15) Phenanthrene	17.322	178	2607	0.027	ng/ul#	87
19) Fluoranthene	19.336	202	2631	0.026	ng/ul#	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030422\
Data File : BN018822.D
Acq On : 03 Mar 2022 12:49
Operator : CG/JU
Sample : N1745-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
H0AA5

Quant Time: Mar 04 01:45:56 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN021822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 18 13:39:55 2022
Response via : Initial Calibration




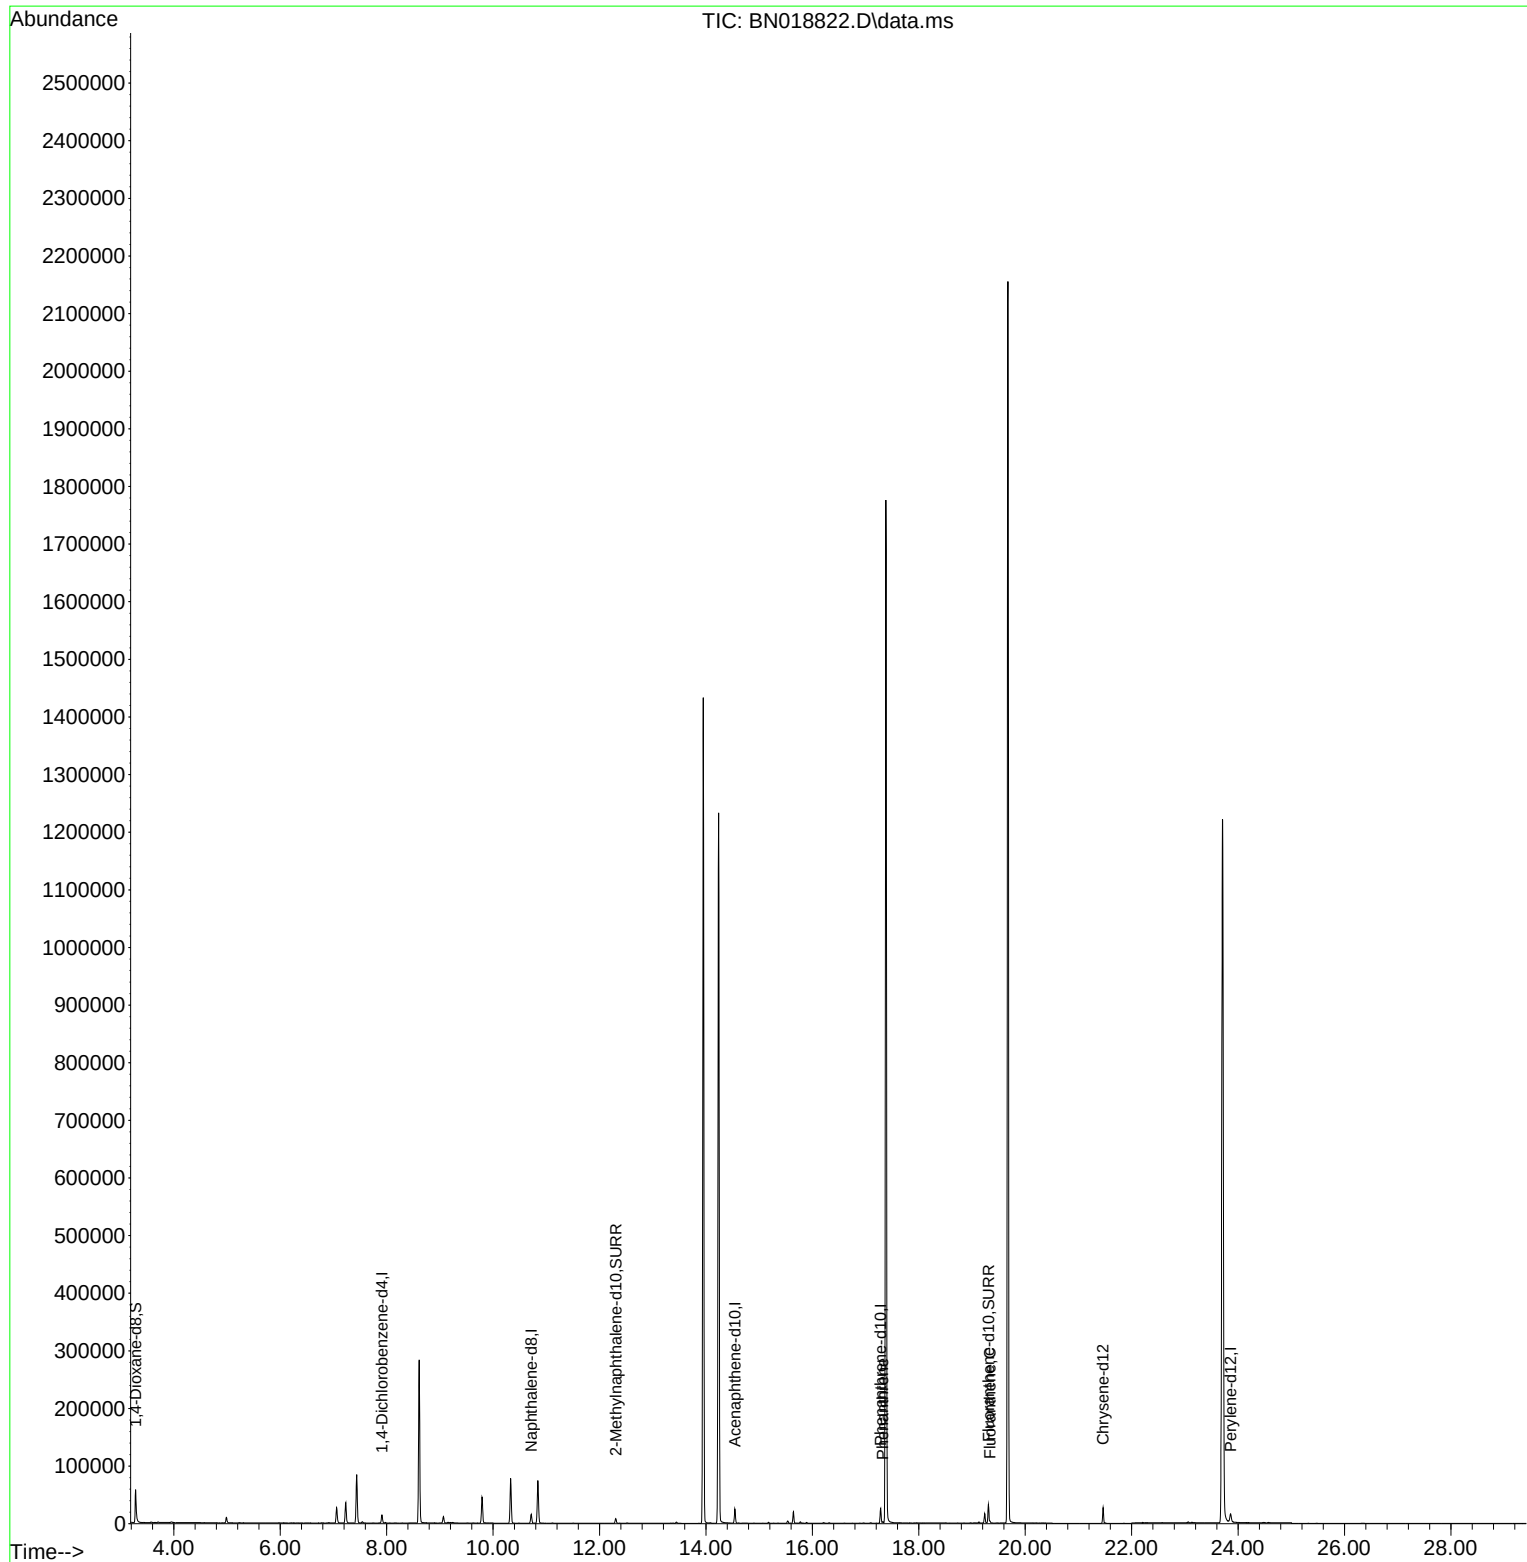


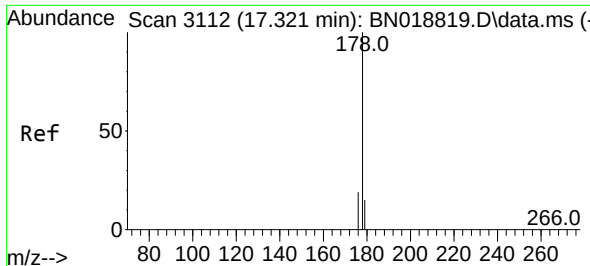

#15
Phenanthrene
Concen: 0.027 ng/ul
RT: 17.322 min Scan# 3112
Delta R.T. -0.007 min
Lab File: BN018822.D
Acq: 03 Mar 2022 12:49

Instrument :
BNA_N
ClientSampleId :
H0AA5

Tgt Ion:178 Resp: 2607
Ion Ratio Lower Upper
178 100
179 21.2 12.2 18.4#
176 24.6 15.4 23.2#

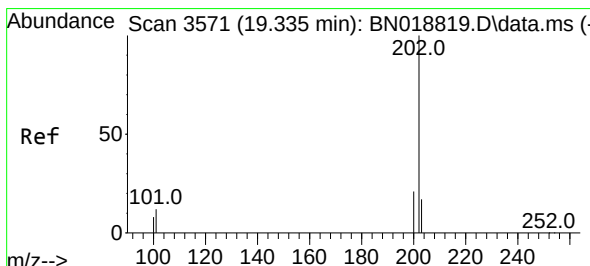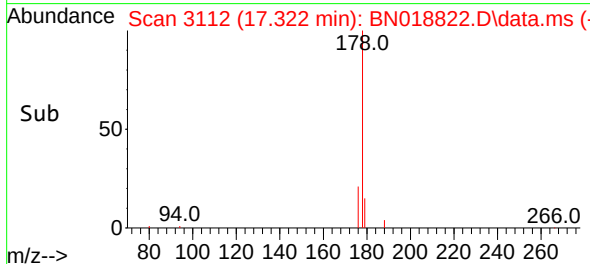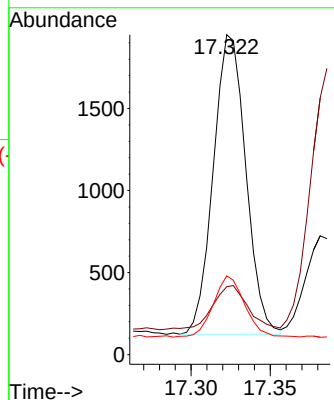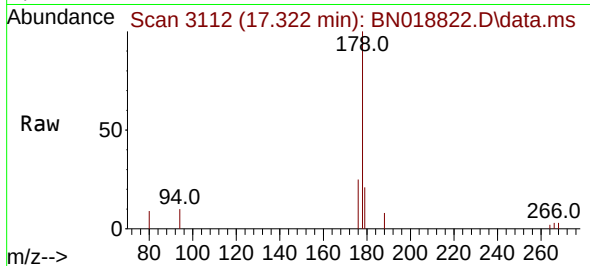

#19
Fluoranthene
Concen: 0.026 ng/ul
RT: 19.336 min Scan# 3571
Delta R.T. -0.007 min
Lab File: BN018822.D
Acq: 03 Mar 2022 12:49

Tgt Ion:202 Resp: 2631
Ion Ratio Lower Upper
202 100
101 16.9 7.5 11.3#
100 15.0 5.4 8.2#

