

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030422\
 Data File : BN018827.D
 Acq On : 03 Mar 2022 15:50
 Operator : CG/JU
 Sample : N1745-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 H0AA4

Quant Time: Mar 04 01:46:29 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN021822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 18 13:39:55 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.913	152	5679	0.400	ng/ul	0.00
4) Naphthalene-d8	10.715	136	16180	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.542	164	10107	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.283	188	22441	0.400	ng/ul	0.00
17) Chrysene-d12	21.465	240	19022	0.400	ng/ul	# 0.00
23) Perylene-d12	23.858	264	16464	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.280	96	26297	4.077	ng/ul	-0.02
6) 2-Methylnaphthalene-d10	12.304	152	8056	0.364	ng/ul	0.00
18) Fluoranthene-d10	19.307	212	26354	0.464	ng/ul	0.00
Target Compounds						
19) Fluoranthene	19.340	202	1688	0.021	ng/ul#	Qvalue 67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030422\
Data File : BN018827.D
Acq On : 03 Mar 2022 15:50
Operator : CG/JU
Sample : N1745-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
H0AA4

Quant Time: Mar 04 01:46:29 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN021822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 18 13:39:55 2022
Response via : Initial Calibration

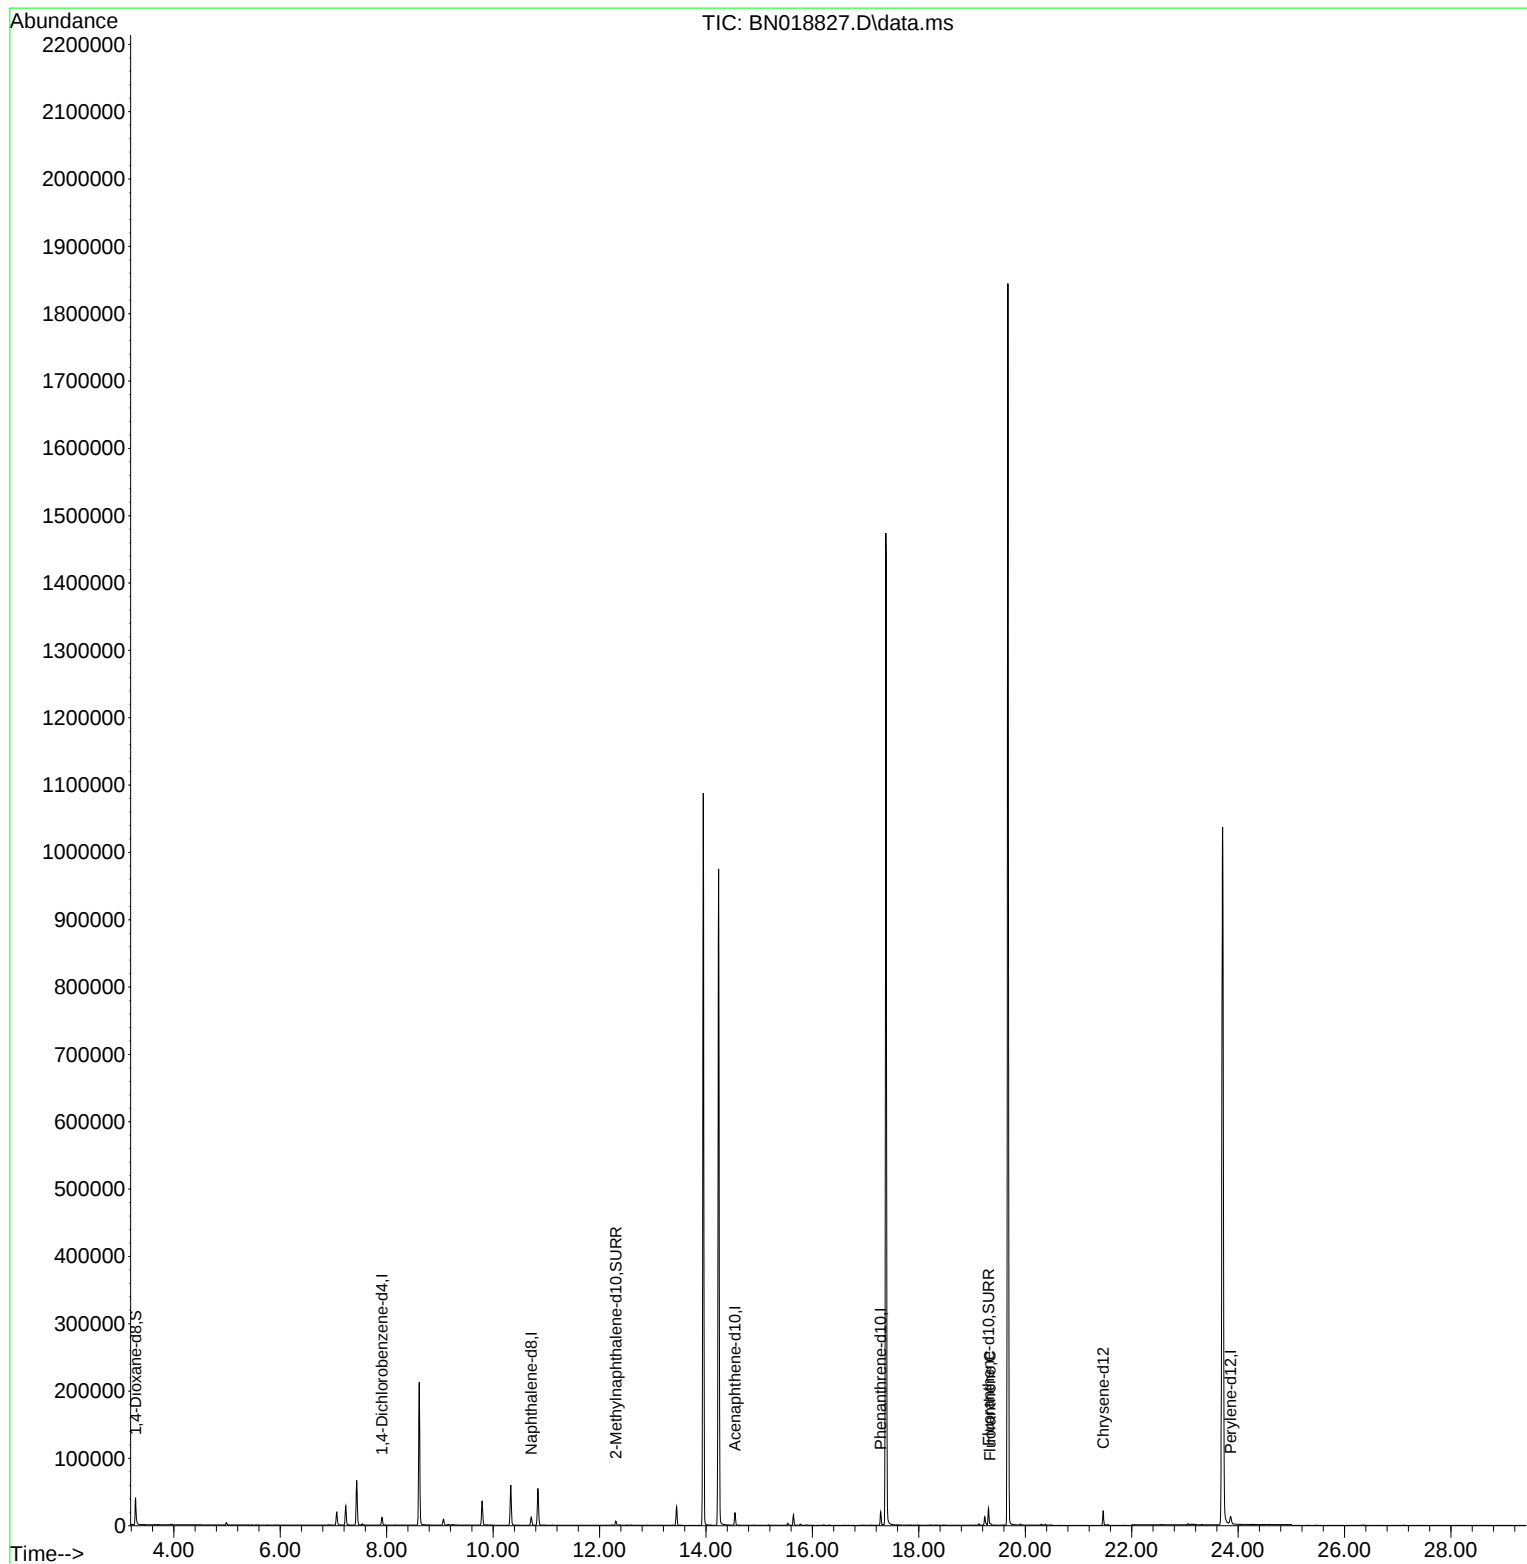

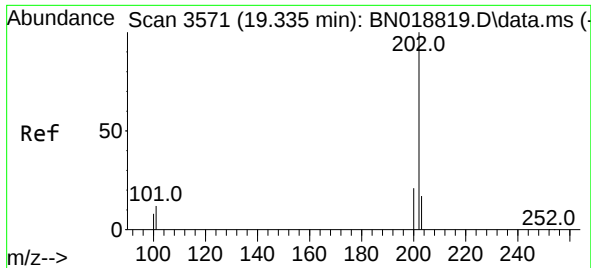

#19

Fluoranthene

Concen: 0.021 ng/ul

RT: 19.340 min Scan# 31

Delta R.T. -0.003 min

Lab File: BN018827.D


Acq: 03 Mar 2022 15:50

Instrument :

BNA_N

ClientSampleId :

H0AA4

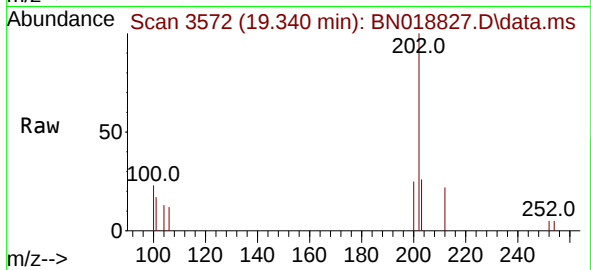

Tgt Ion:202 Resp: 1688

Ion Ratio Lower Upper

202 100

101 17.4 7.5 11.3#

100 23.2 5.4 8.2#

