

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030422\
 Data File : BN018829.D
 Acq On : 03 Mar 2022 17:03
 Operator : CG/JU
 Sample : N1745-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 H0AA3

Quant Time: Mar 04 01:46:44 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN021822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 18 13:39:55 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.913	152	5643	0.400	ng/ul	0.00
4) Naphthalene-d8	10.715	136	16036	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.543	164	9904	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.284	188	22017	0.400	ng/ul	0.00
17) Chrysene-d12	21.463	240	18885	0.400	ng/ul	# 0.00
23) Perylene-d12	23.857	264	16112	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.280	96	25591	3.993	ng/ul	-0.02
6) 2-Methylnaphthalene-d10	12.305	152	7316	0.334	ng/ul	0.00
18) Fluoranthene-d10	19.309	212	24759	0.439	ng/ul	0.00
Target Compounds						
19) Fluoranthene	19.341	202	1704	0.021	ng/ul#	Qvalue 76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030422\
Data File : BN018829.D
Acq On : 03 Mar 2022 17:03
Operator : CG/JU
Sample : N1745-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
H0AA3

Quant Time: Mar 04 01:46:44 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN021822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 18 13:39:55 2022
Response via : Initial Calibration

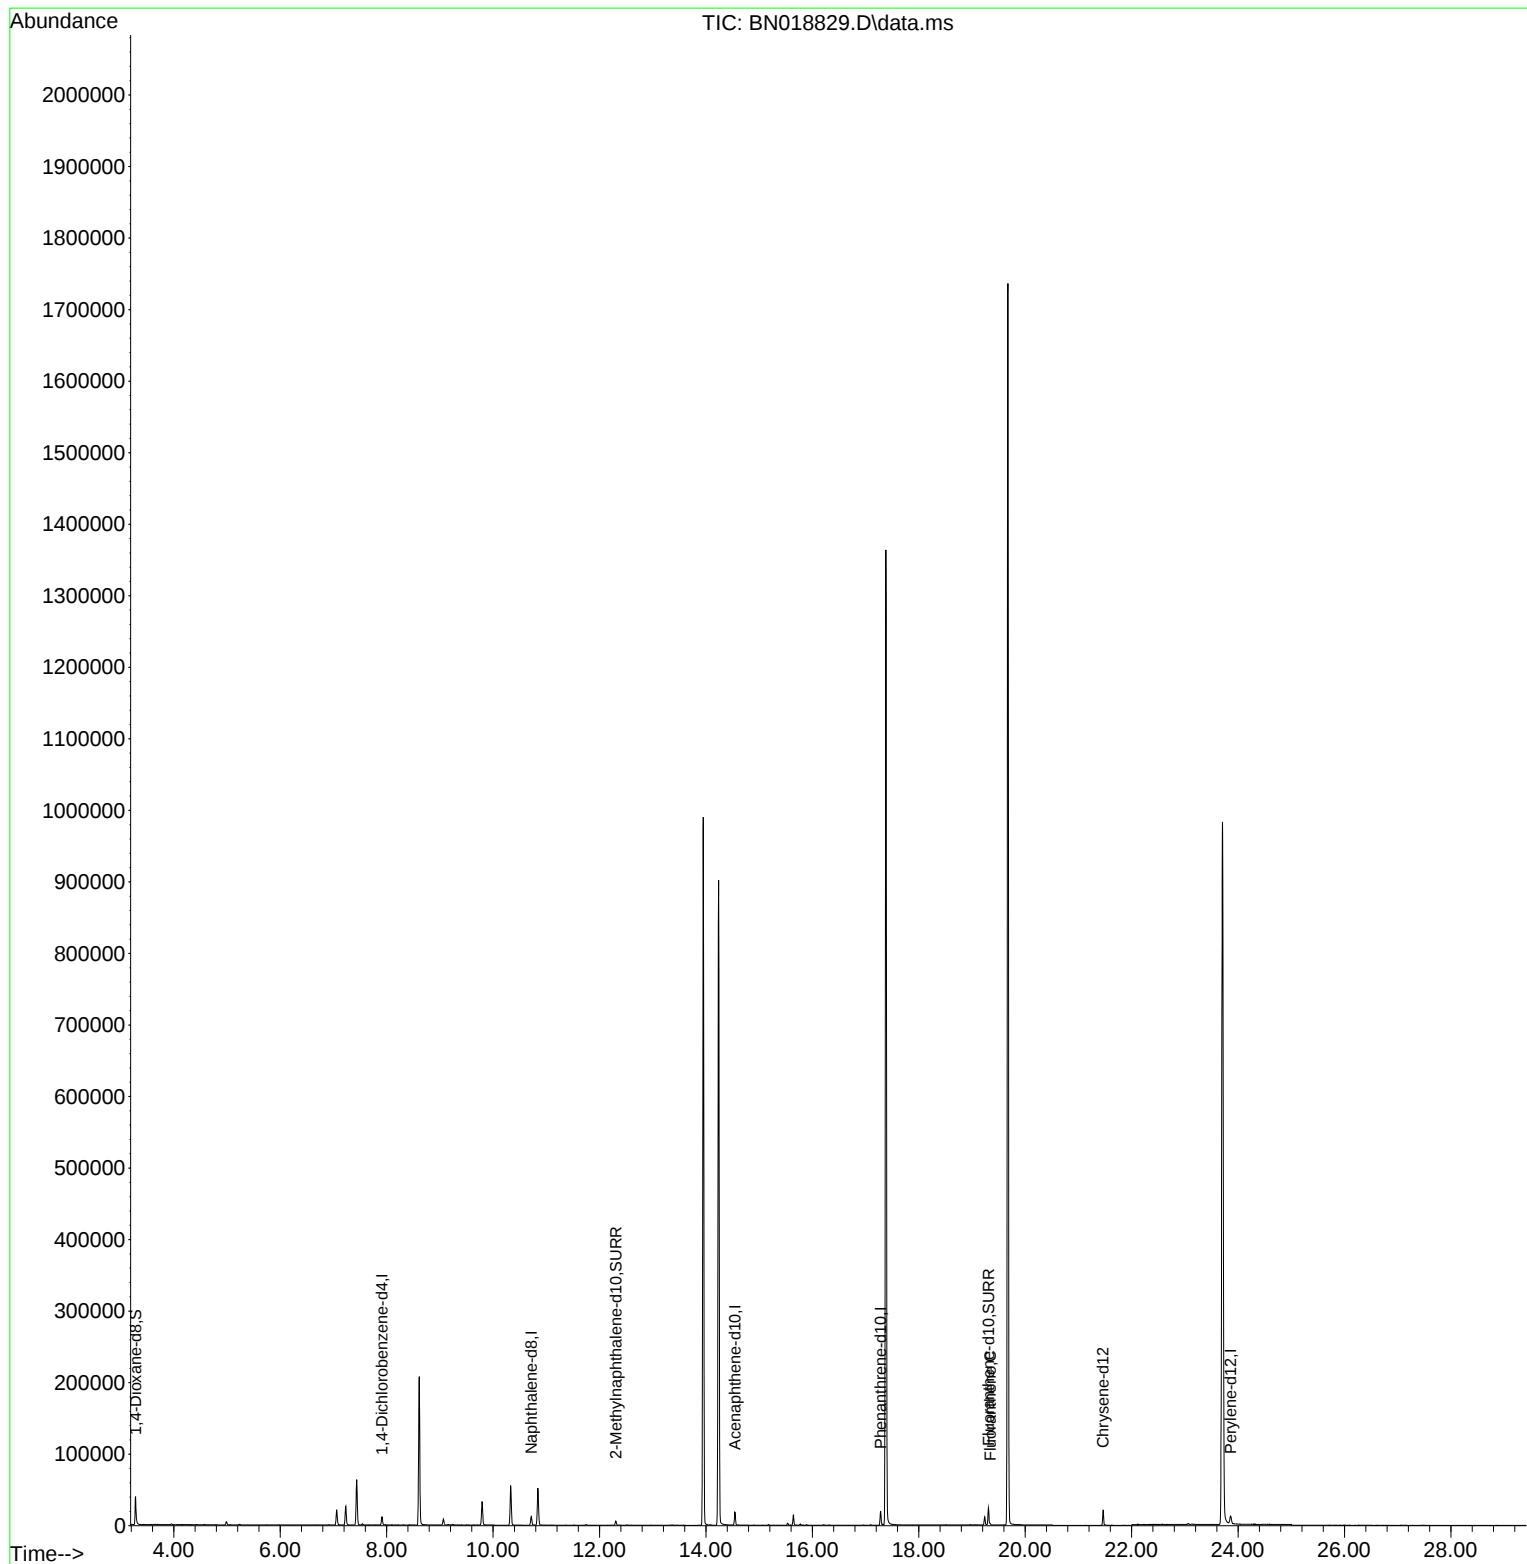

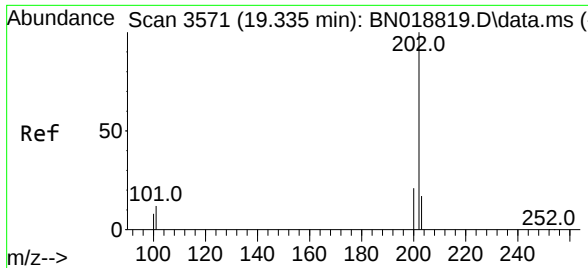

#19
 Fluoranthene
 Concen: 0.021 ng/ul
 RT: 19.341 min Scan# 31
 Delta R.T. -0.002 min
 Lab File: BN018829.D
 Acq: 03 Mar 2022 17:03

Instrument :
 BNA_N
 ClientSampleId :
 H0AA3

Tgt Ion:202 Resp: 1704
 Ion Ratio Lower Upper
 202 100
 101 16.8 7.5 11.3#
 100 17.0 5.4 8.2#

