

Data Path : Z:\HPCHEM1\BNA_N\DATA\BN030518\
 Data File : BN000247.D
 Acq On : 05 Mar 2018 16:17
 Operator : JU/SJ
 Sample : MDL-SIM-S-02
 Misc : 0.07 PPM
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MDL-SIM-S-02

Quant Time: Mar 05 16:58:33 2018
 Quant Method : Z:\HPCHEM1\BNA_N\Methods\SOM-EPA-SIM-BN030218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 05 15:16:04 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.45	152	3654	0.40	ng/ul	0.00
2) Naphthalene-d8	11.29	136	11875	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.06	164	5121	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.78	188	11830	0.40	ng/ul	0.00
16) Chrysene-d12	21.89	240	6790	0.40	ng/ul	0.00
20) Perylene-d12	24.36	264	5480	0.40	ng/ul	-0.02
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.85	152	6050	0.39	ng/ul	0.00
14) Fluoranthene-d10	19.77	212	10665	0.39	ng/ul	0.00
Target Compounds				Qvalue		
3) Naphthalene	11.34	128	2787	0.073	ng/ul#	91
5) 2-Methylnaphthalene	12.92	142	1706	0.071	ng/ul	99
7) Acenaphthylene	14.79	152	1744	0.068	ng/ul	97
8) Acenaphthene	15.12	153	1732	0.070	ng/ul#	94
9) Fluorene	16.10	166	1845	0.069	ng/ul	92
11) Pentachlorophenol	17.42	266	100	0.042	ng/ul#	76
12) Phenanthrene	17.82	178	3395	0.070	ng/ul#	88
13) Anthracene	17.91	178	2343	0.065	ng/ul#	93
15) Fluoranthene	19.80	202	3255	0.069	ng/ul	62
17) Pyrene	20.15	202	3150	0.079	ng/ul#	55
18) Benzo(a)anthracene	21.88	228	1860	0.070	ng/ul#	84
19) Chrysene	21.93	228	2937	0.081	ng/ul	96
21) Benzo(b)fluoranthene	23.61	252	2376	0.072	ng/ul	82
22) Benzo(k)fluoranthene	23.66	252	2126	0.068	ng/ul#	75
23) Benzo(a)pyrene	24.26	252	1785	0.069	ng/ul#	73
24) Indeno(1,2,3-cd)pyrene	26.91	276	1922	0.066	ng/ul#	79
25) Dibenzo(a,h)anthracene	26.93	278	1346	0.064	ng/ul#	66
26) Benzo(g,h,i)perylene	27.70	276	2051	0.071	ng/ul#	73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_N\DATA\BN030518\
Data File : BN000247.D
Acq On : 05 Mar 2018 16:17
Operator : JU/SJ
Sample : MDL-SIM-S-02
Misc : 0.07 PPM
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MDL-SIM-S-02

Quant Time: Mar 05 16:58:33 2018
Quant Method : Z:\HPCHEM1\BNA_N\Methods\SOM-EPA-SIM-BN030218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 05 15:16:04 2018
Response via : Initial Calibration

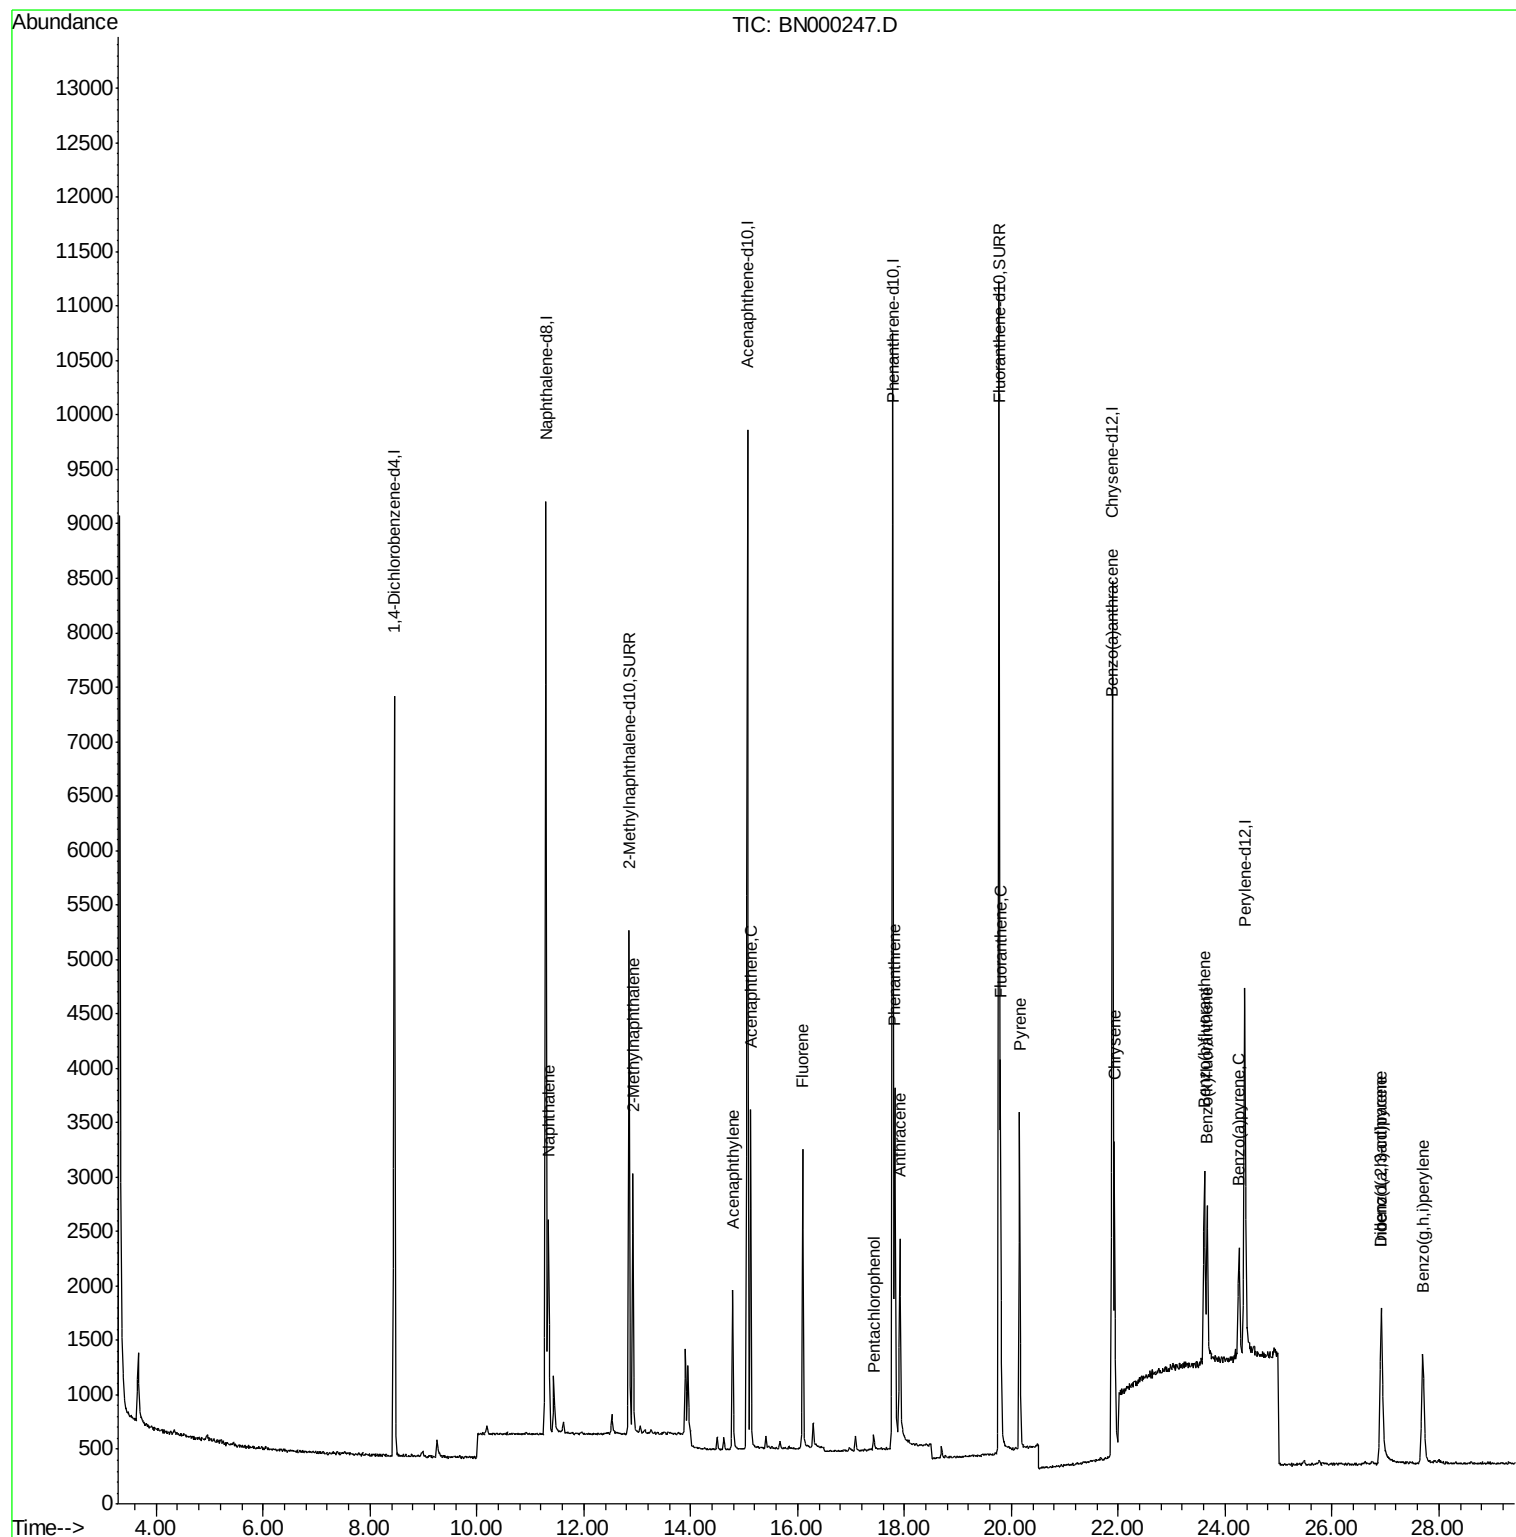



#3

Naphthalene

Concen: 0.073 ng/ul

RT: 11.34 min Scan# 2546

Delta R.T. 0.00 min

Lab File: BN000247.D

Acq: 05 Mar 2018 16:17

Instrument :

BNA_N

ClientSampleId :

MDL-SIM-S-02


Tgt Ion:128 Resp: 2787

Ion Ratio Lower Upper

128 100

129 13.9 11.3 16.9




127 15.7 4.0 6.0#

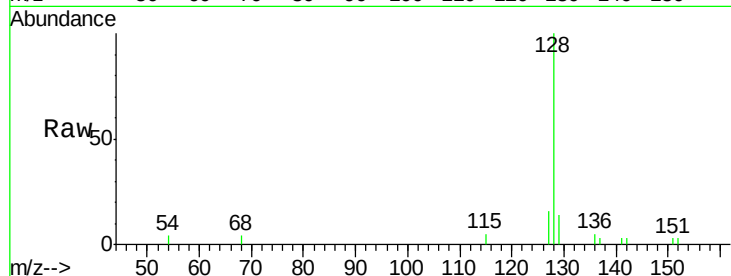

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

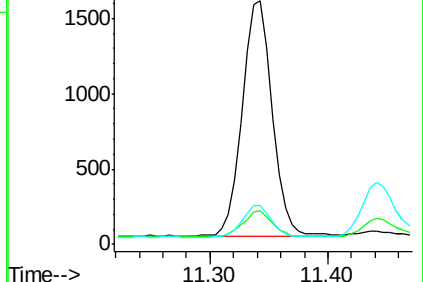

#5

2-Methylnaphthalene

Concen: 0.071 ng/ul

RT: 12.92 min Scan# 2833

Delta R.T. -0.00 min

Lab File: BN000247.D


Acq: 05 Mar 2018 16:17

Tgt Ion:142 Resp: 1706

Ion Ratio Lower Upper



142 100


141 90.1 72.6 108.8



Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

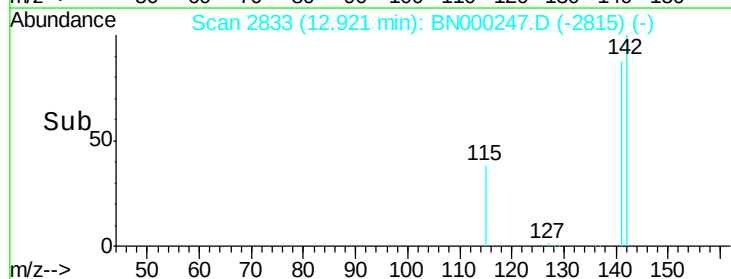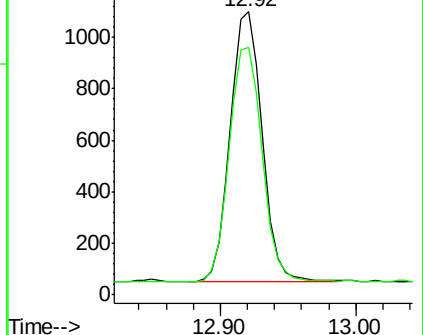



#7

Acenaphthylene

Concen: 0.068 ng/ul

RT: 14.79 min Scan# 3199

Delta R.T. -0.00 min

Lab File: BN000247.D

Acq: 05 Mar 2018 16:17

Instrument :

BNA_N

ClientSampleId :

MDL-SIM-S-02


Tgt Ion:152 Resp: 1744

Ion Ratio Lower Upper

152 100

151 23.3 17.1 25.7




153 17.0 12.8 19.2



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

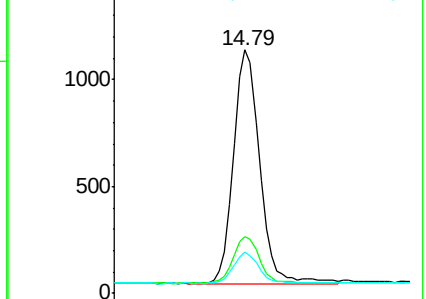

#8

Acenaphthene

Concen: 0.070 ng/ul

RT: 15.12 min Scan# 3272

Delta R.T. 0.00 min

Lab File: BN000247.D

Acq: 05 Mar 2018 16:17


Tgt Ion:153 Resp: 1732

Ion Ratio Lower Upper

153 100

152 54.1 36.0 54.0#



154 88.7 72.0 108.0




Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

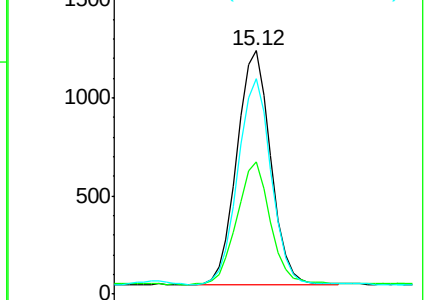



#9

Fluorene

Concen: 0.069 ng/ul

RT: 16.10 min Scan# 3482

Delta R.T. -0.00 min

Lab File: BN000247.D

Acq: 05 Mar 2018 16:17

Instrument :

BNA_N

ClientSampleId :

MDL-SIM-S-02





Tgt Ion:166 Resp: 1845

Ion Ratio Lower Upper

166 100

165 100.6 73.4 110.2

167 16.2 14.6 22.0

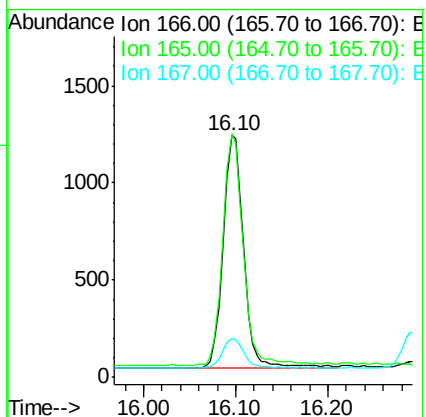

#11

Pentachlorophenol

Concen: 0.042 ng/ul

RT: 17.42 min Scan# 3788

Delta R.T. -0.00 min

Lab File: BN000247.D

Acq: 05 Mar 2018 16:17




Tgt Ion:266 Resp: 100


Ion Ratio Lower Upper

266 100

264 76.0 47.9 71.9#

268 83.0 49.8 74.8#

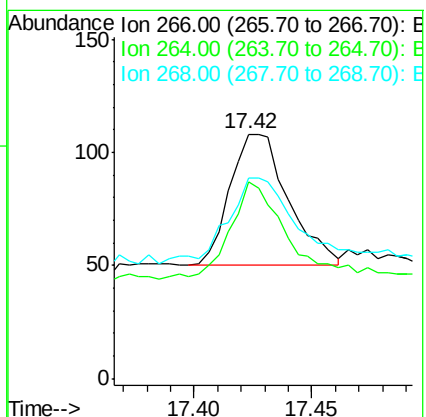

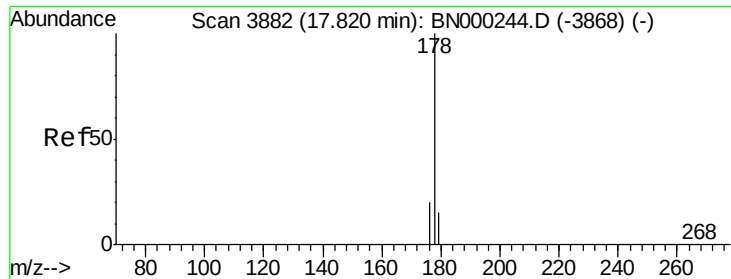

#12

Phenanthrene

Concen: 0.070 ng/ul

RT: 17.82 min Scan# 3882

Delta R.T. -0.00 min

Lab File: BN000247.D

Acq: 05 Mar 2018 16:17

Instrument :

BNA_N

ClientSampleId :

MDL-SIM-S-02





Tgt Ion:178 Resp: 3395

Ion Ratio Lower Upper

178 100

179 17.7 18.4 27.6#

176 22.6 13.6 20.4#

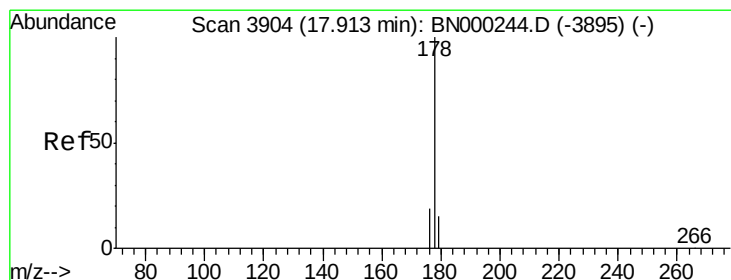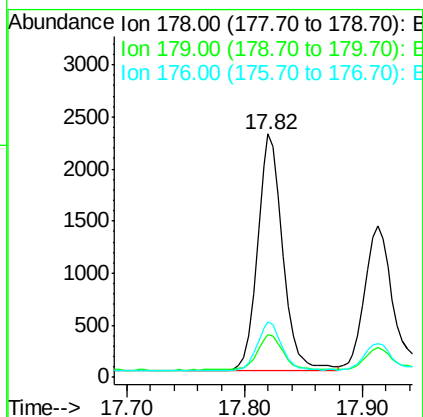

#13

Anthracene

Concen: 0.065 ng/ul

RT: 17.91 min Scan# 3904

Delta R.T. 0.00 min

Lab File: BN000247.D

Acq: 05 Mar 2018 16:17




Tgt Ion:178 Resp: 2343


Ion Ratio Lower Upper

178 100

179 19.7 18.1 27.1

176 22.4 14.7 22.1#

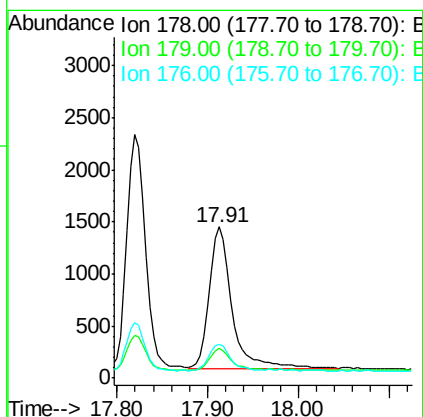

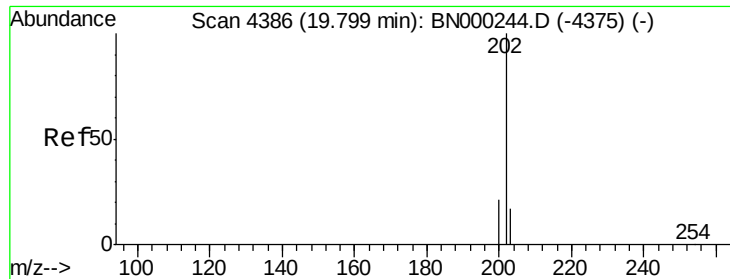

#15

Fluoranthene

Concen: 0.069 ng/ul

RT: 19.80 min Scan# 4386

Delta R.T. -0.00 min

Lab File: BN000247.D

Acq: 05 Mar 2018 16:17

Instrument :

BNA_N

ClientSampleId :

MDL-SIM-S-02


Tgt Ion:202 Resp: 3255

Ion Ratio Lower Upper

202 100

101 0.0 0.0 30.3




100 0.0 0.0 39.5

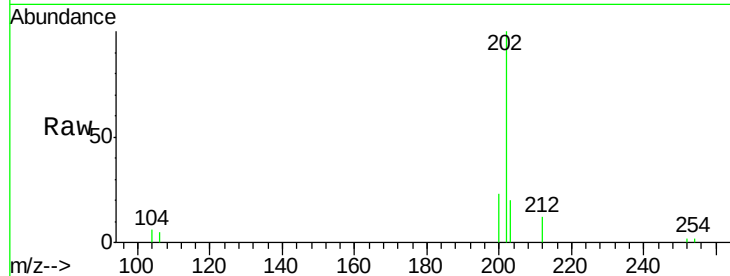

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

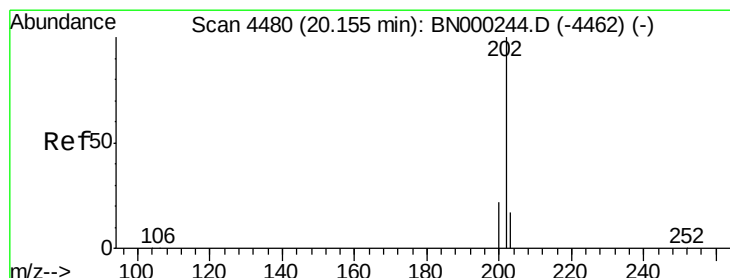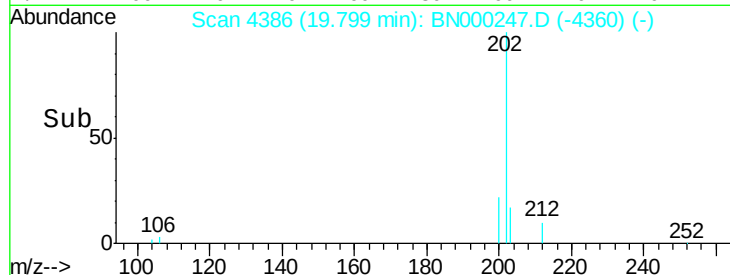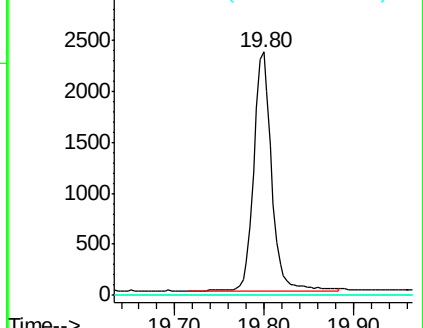

#17

Pyrene

Concen: 0.079 ng/ul

RT: 20.15 min Scan# 4480

Delta R.T. -0.00 min

Lab File: BN000247.D

Acq: 05 Mar 2018 16:17


Tgt Ion:202 Resp: 3150

Ion Ratio Lower Upper

202 100

101 0.0 18.2 27.4#



100 0.0 15.6 23.4#

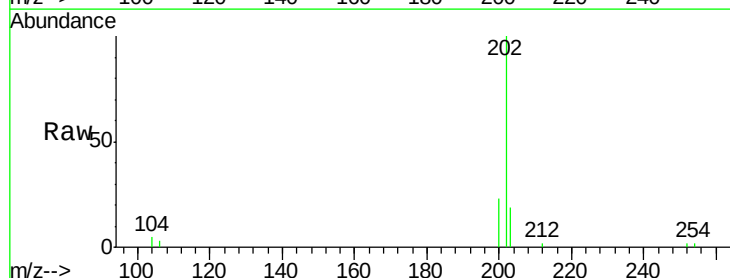


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

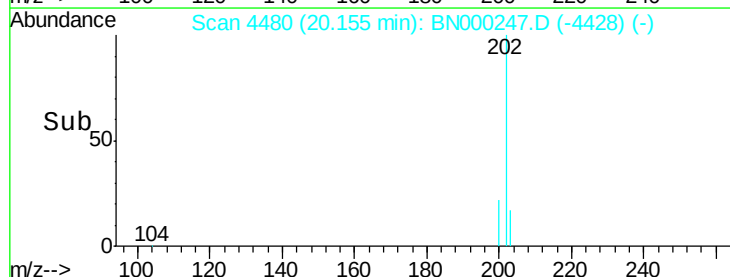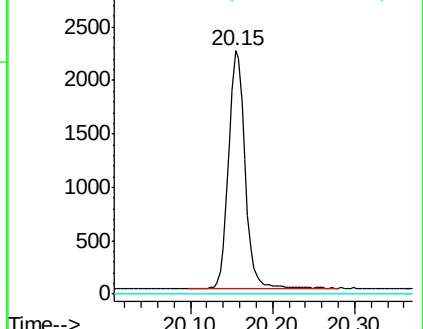

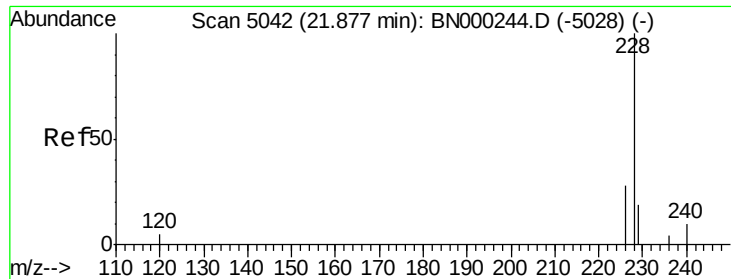

#18

Benzo(a)anthracene

Concen: 0.070 ng/ul

RT: 21.88 min Scan# 5042

Delta R.T. -0.01 min

Lab File: BN000247.D

Acq: 05 Mar 2018 16:17

Instrument :

BNA_N

ClientSampleId :

MDL-SIM-S-02





Tgt Ion:228 Resp: 1860

Ion Ratio Lower Upper

228 100

229 21.8 22.8 34.2#

226 31.0 17.0 25.6#

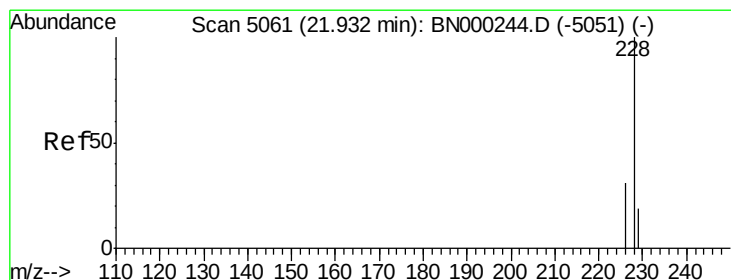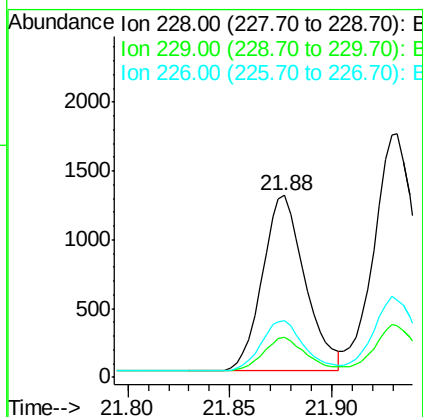

#19

Chrysene

Concen: 0.081 ng/ul

RT: 21.93 min Scan# 5061

Delta R.T. -0.00 min

Lab File: BN000247.D

Acq: 05 Mar 2018 16:17




Tgt Ion:228 Resp: 2937


Ion Ratio Lower Upper

228 100

226 32.0 23.4 35.0

229 21.2 17.7 26.5

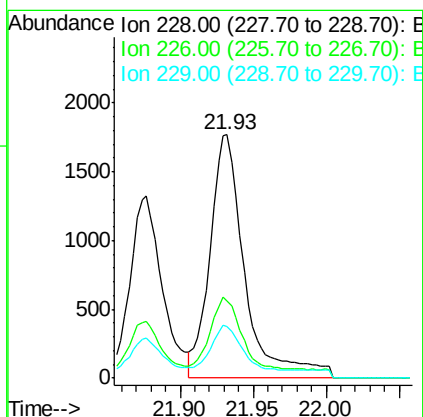

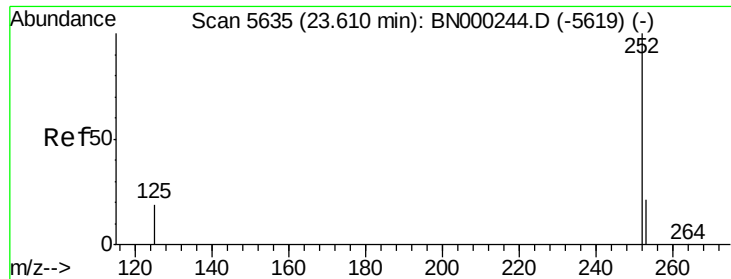

#21

Benzo(b)fluoranthene

Concen: 0.072 ng/ul

RT: 23.61 min Scan# 5634

Delta R.T. -0.02 min

Lab File: BN000247.D

Acq: 05 Mar 2018 16:17

Instrument :

BNA_N

ClientSampleId :

MDL-SIM-S-02


Tgt Ion:252 Resp: 2376

Ion Ratio Lower Upper

252 100

253 36.8 0.0 64.2




125 33.7 0.0 35.0



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

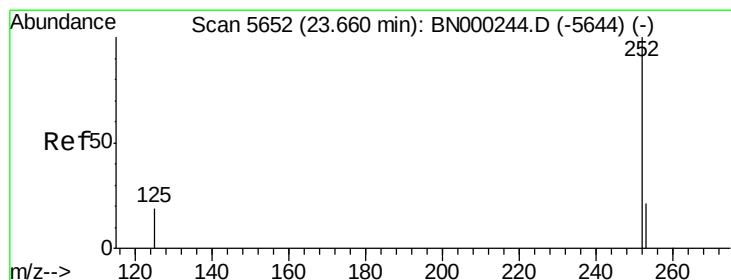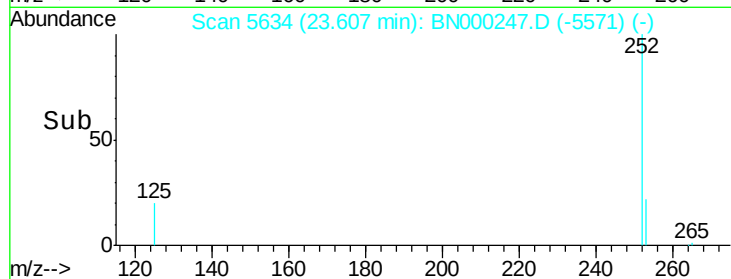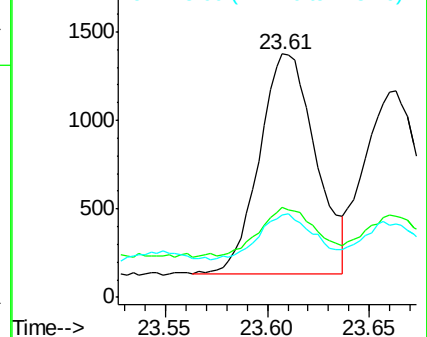

#22

Benzo(k)fluoranthene

Concen: 0.068 ng/ul

RT: 23.66 min Scan# 5653

Delta R.T. -0.01 min

Lab File: BN000247.D

Acq: 05 Mar 2018 16:17


Tgt Ion:252 Resp: 2126

Ion Ratio Lower Upper

252 100

253 39.0 24.5 36.7#



125 35.8 13.7 20.5#

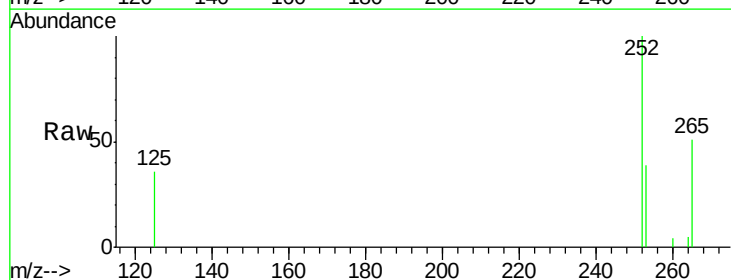


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

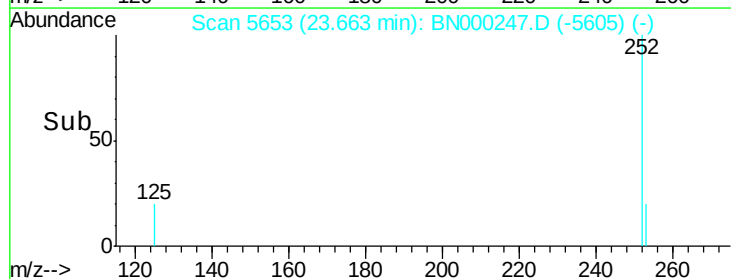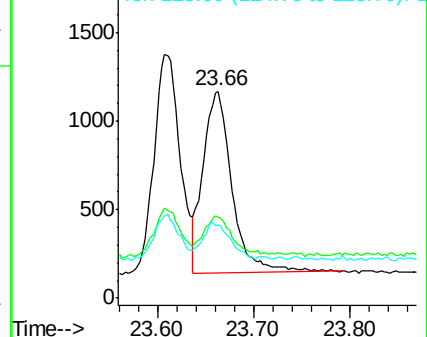

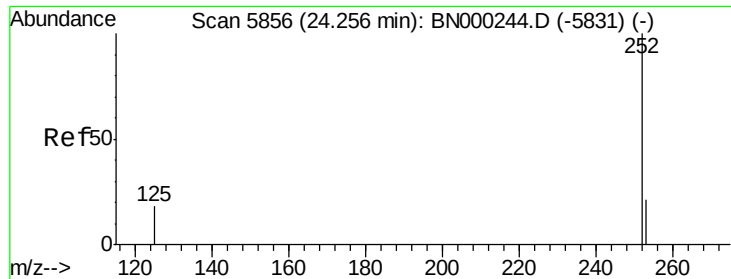

#23

Benzo(a)pyrene

Concen: 0.069 ng/uL

RT: 24.26 min Scan# 5857

Delta R.T. -0.01 min

Lab File: BN000247.D

Acq: 05 Mar 2018 16:17

Instrument :

BNA_N

ClientSampled :

MDL-SIM-S-02


Tgt Ion: 252 Resp: 1785

Ion Ratio Lower Upper

252 100

253 45.5 28.5 42.7#




125 42.9 18.1 27.1#



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

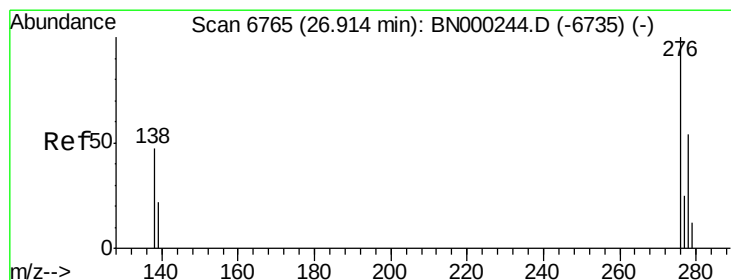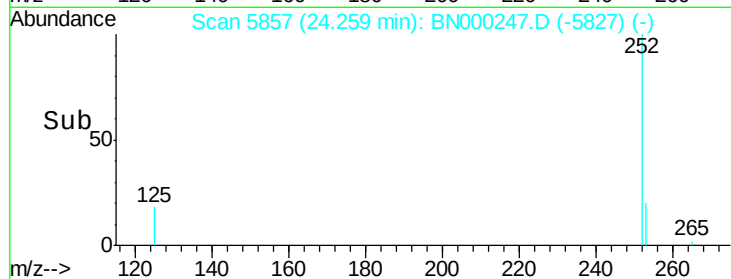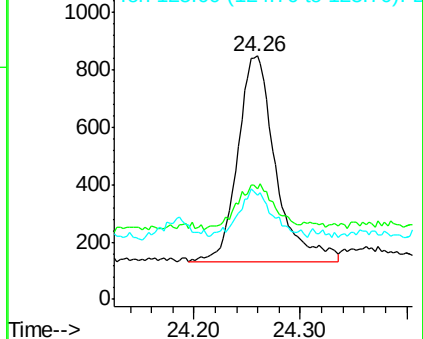

#24

Indeno(1,2,3-cd)pyrene

Concen: 0.066 ng/uL

RT: 26.91 min Scan# 6764

Delta R.T. -0.03 min

Lab File: BN000247.D

Acq: 05 Mar 2018 16:17


Tgt Ion: 276 Resp: 1922

Ion Ratio Lower Upper

276 100

138 45.9 28.0 42.0#



227 0.0 8.0 12.0#

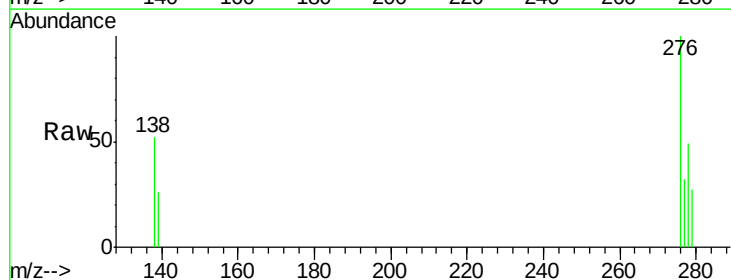


Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 227.00 (226.70 to 227.70): E

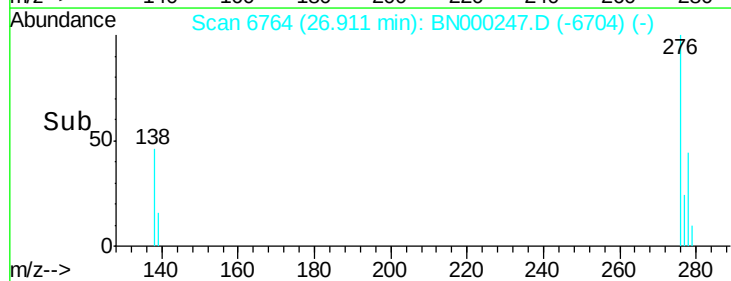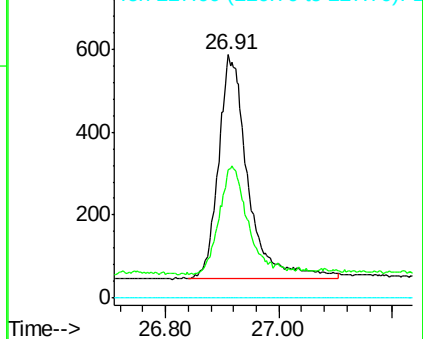

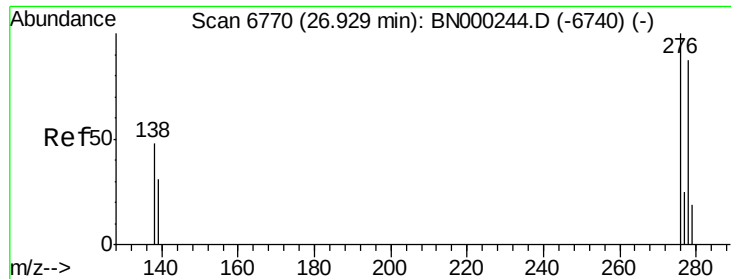

#25

Dibenzo(a,h)anthracene

Concen: 0.064 ng/ul

RT: 26.93 min Scan# 6770

Delta R.T. -0.02 min

Lab File: BN000247.D


Acq: 05 Mar 2018 16:17

Instrument :

BNA_N

ClientSampleId :

MDL-SIM-S-02






Tgt Ion:278 Resp: 1346

Ion Ratio Lower Upper

278 100

139 45.0 17.4 26.0#

279 46.0 25.9 38.9#

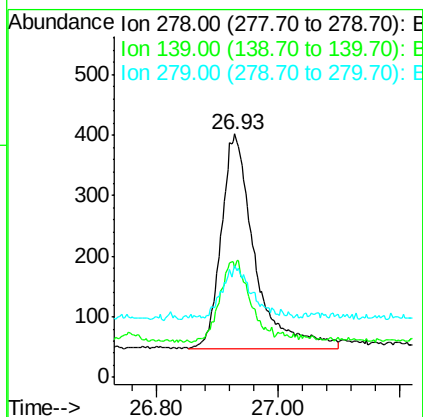

#26

Benzo(g,h,i)perylene

Concen: 0.071 ng/ul

RT: 27.70 min Scan# 7034

Delta R.T. -0.02 min

Lab File: BN000247.D

Acq: 05 Mar 2018 16:17

Tgt Ion:276 Resp: 2051

Ion Ratio Lower Upper

276 100

138 50.0 21.8 32.8#

277 30.3 20.5 30.7

