
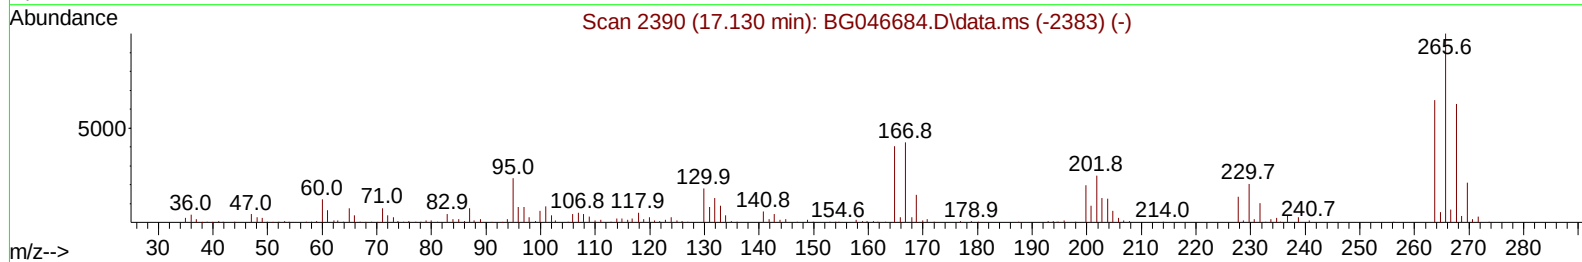
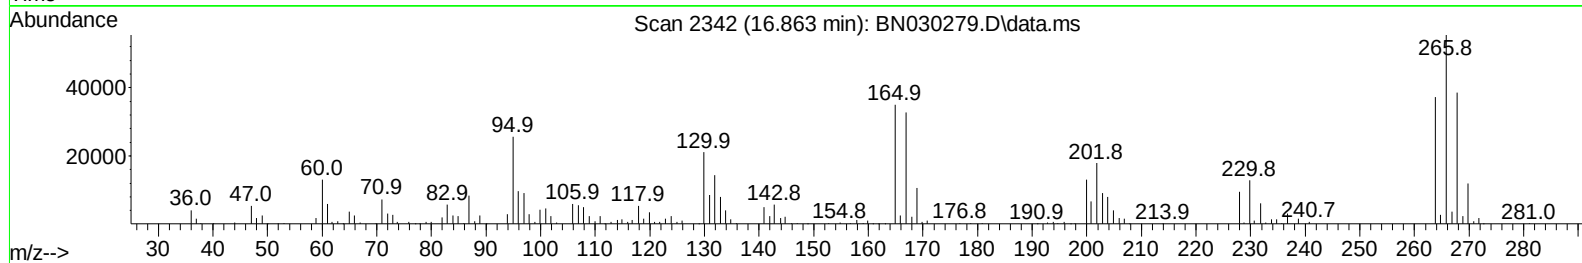


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN030524\  
Data File : BN030279.D  
Acq On : 06 Mar 2024 00:50  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 41 Sample Multiplier: 1

Quant Time: Mar 06 02:57:13 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Mar 06 02:54:35 2024  
Response via : Initial Calibration

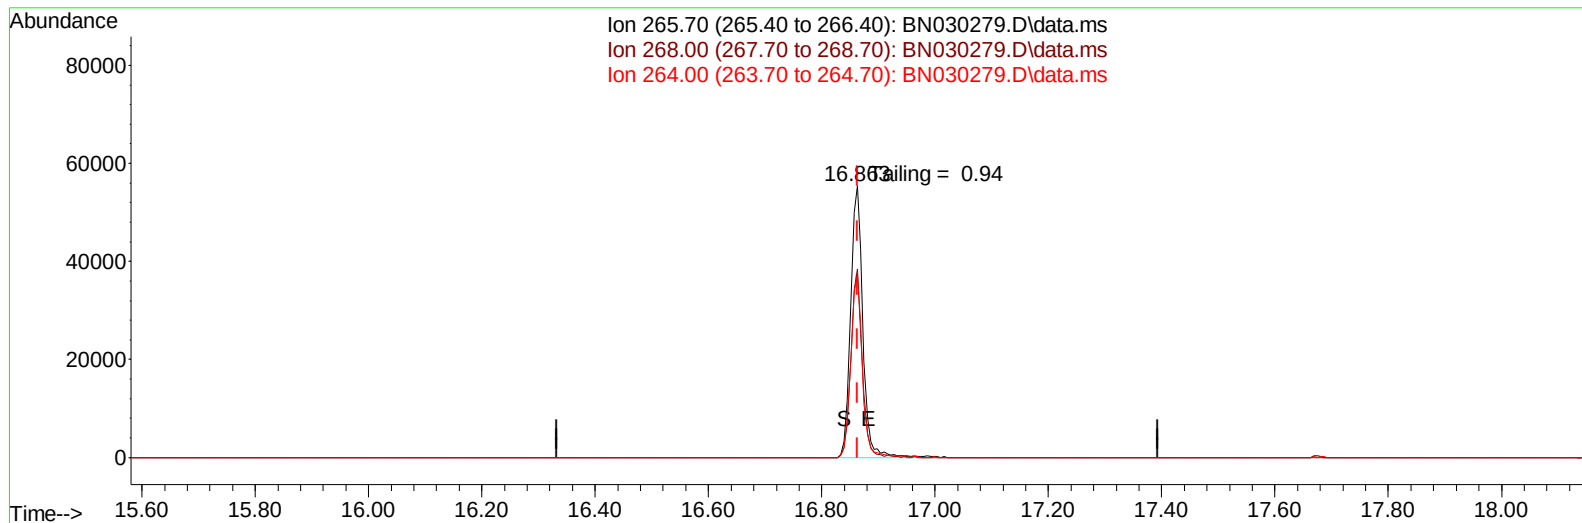




TIC: BN030279.D\data.ms

**(70) Pentachlorophenol (C)****16.863min (-0.000) 17086.68 ng****response 83137**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 69.44  |
| 264.00 | 61.60  | 67.30  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN030524\  
Data File : BN030279.D  
Acq On : 06 Mar 2024 00:50  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 41 Sample Multiplier: 1

Quant Time: Mar 06 02:57:13 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Mar 06 02:54:35 2024  
Response via : Initial Calibration

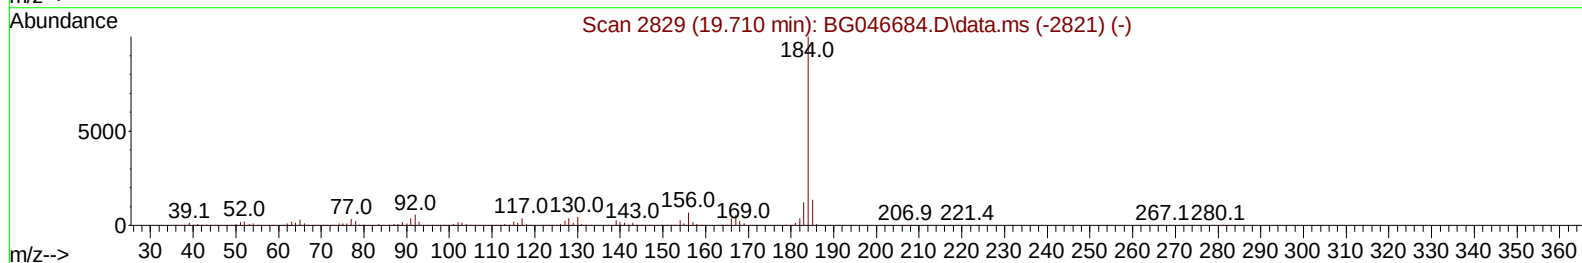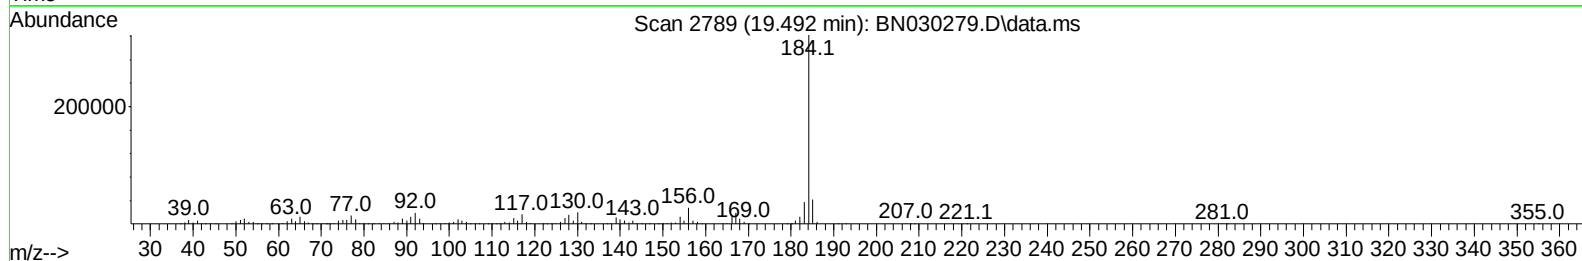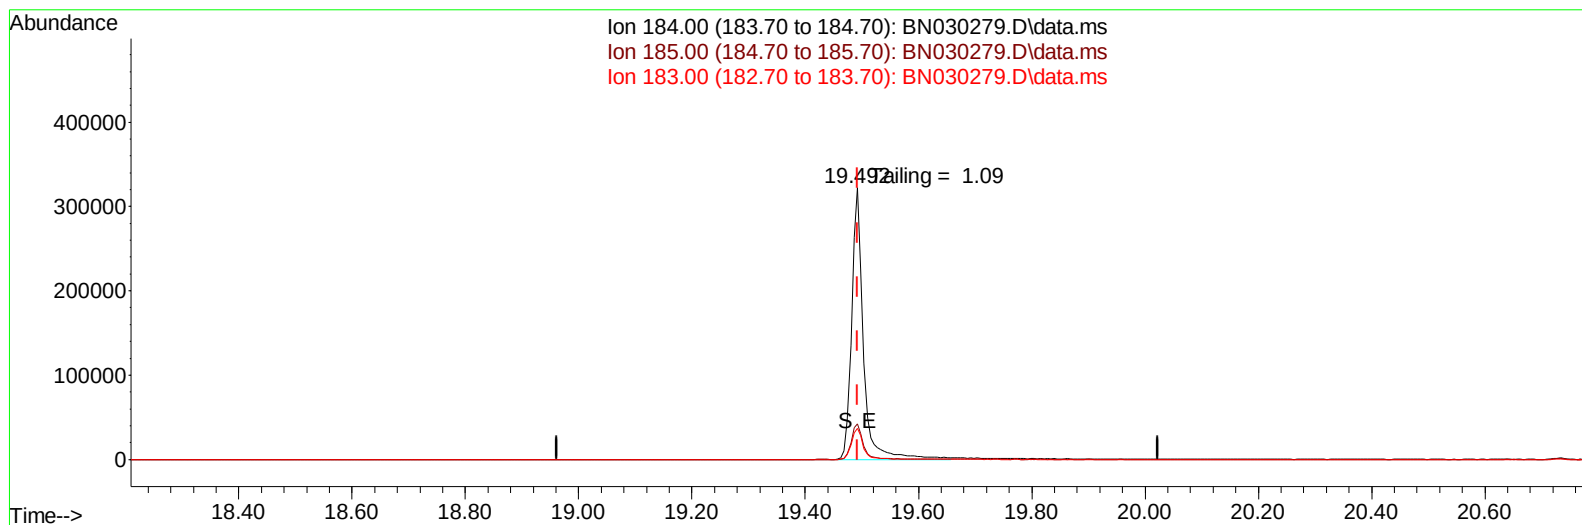

TIC: BN030279.D\data.ms

**(77) Benzidine**

19.492min (-0.000) 0.00 ng

response 469240

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 13.03  |
| 183.00 | 13.20  | 11.52  |
| 0.00   | 0.00   | 0.00   |